

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
 Data File : VW030976.D
 Acq On : 08 Nov 2024 17:39
 Operator : SY/MD
 Sample : P4724-21
 Misc : 6.20g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 08 22:08:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 08 22:04:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	552964	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	475100	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	189073	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	138999	15.327	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	61.320%		
7) Chloroethane-d5	2.905	69	109497	15.742	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	62.960%		
11) 1,1-Dichloroethene-d2	4.027	65	61896	16.540	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.160%		
21) 2-Butanone-d5	7.075	46	76062	50.964	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.920%		
24) Chloroform-d	7.654	84	304867	18.702	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	74.800%		
26) 1,2-Dichloroethane-d4	8.306	65	163328	20.151	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	80.600%		
32) Benzene-d6	8.276	84	567734	19.235	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.960%		
36) 1,2-Dichloropropane-d6	9.276	67	183405	21.079	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.320%		
41) Toluene-d8	10.324	98	453252	17.120	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	68.480%		
43) trans-1,3-Dichloroprop...	10.580	79	68747	19.492	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.960%		
47) 2-Hexanone-d5	10.922	63	59153	52.457	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	104.920%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	151609	25.010	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	100.040%		
66) 1,2-Dichlorobenzene-d4	13.848	152	147789	21.459	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	85.840%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4450	0.389	ug/L	# 41


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
Data File : VW030976.D
Acq On : 08 Nov 2024 17:39
Operator : SY/MD
Sample : P4724-21
Misc : 6.20g/10mL/MSVOA_W/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 08 22:08:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 08 22:04:34 2024
Response via : Initial Calibration

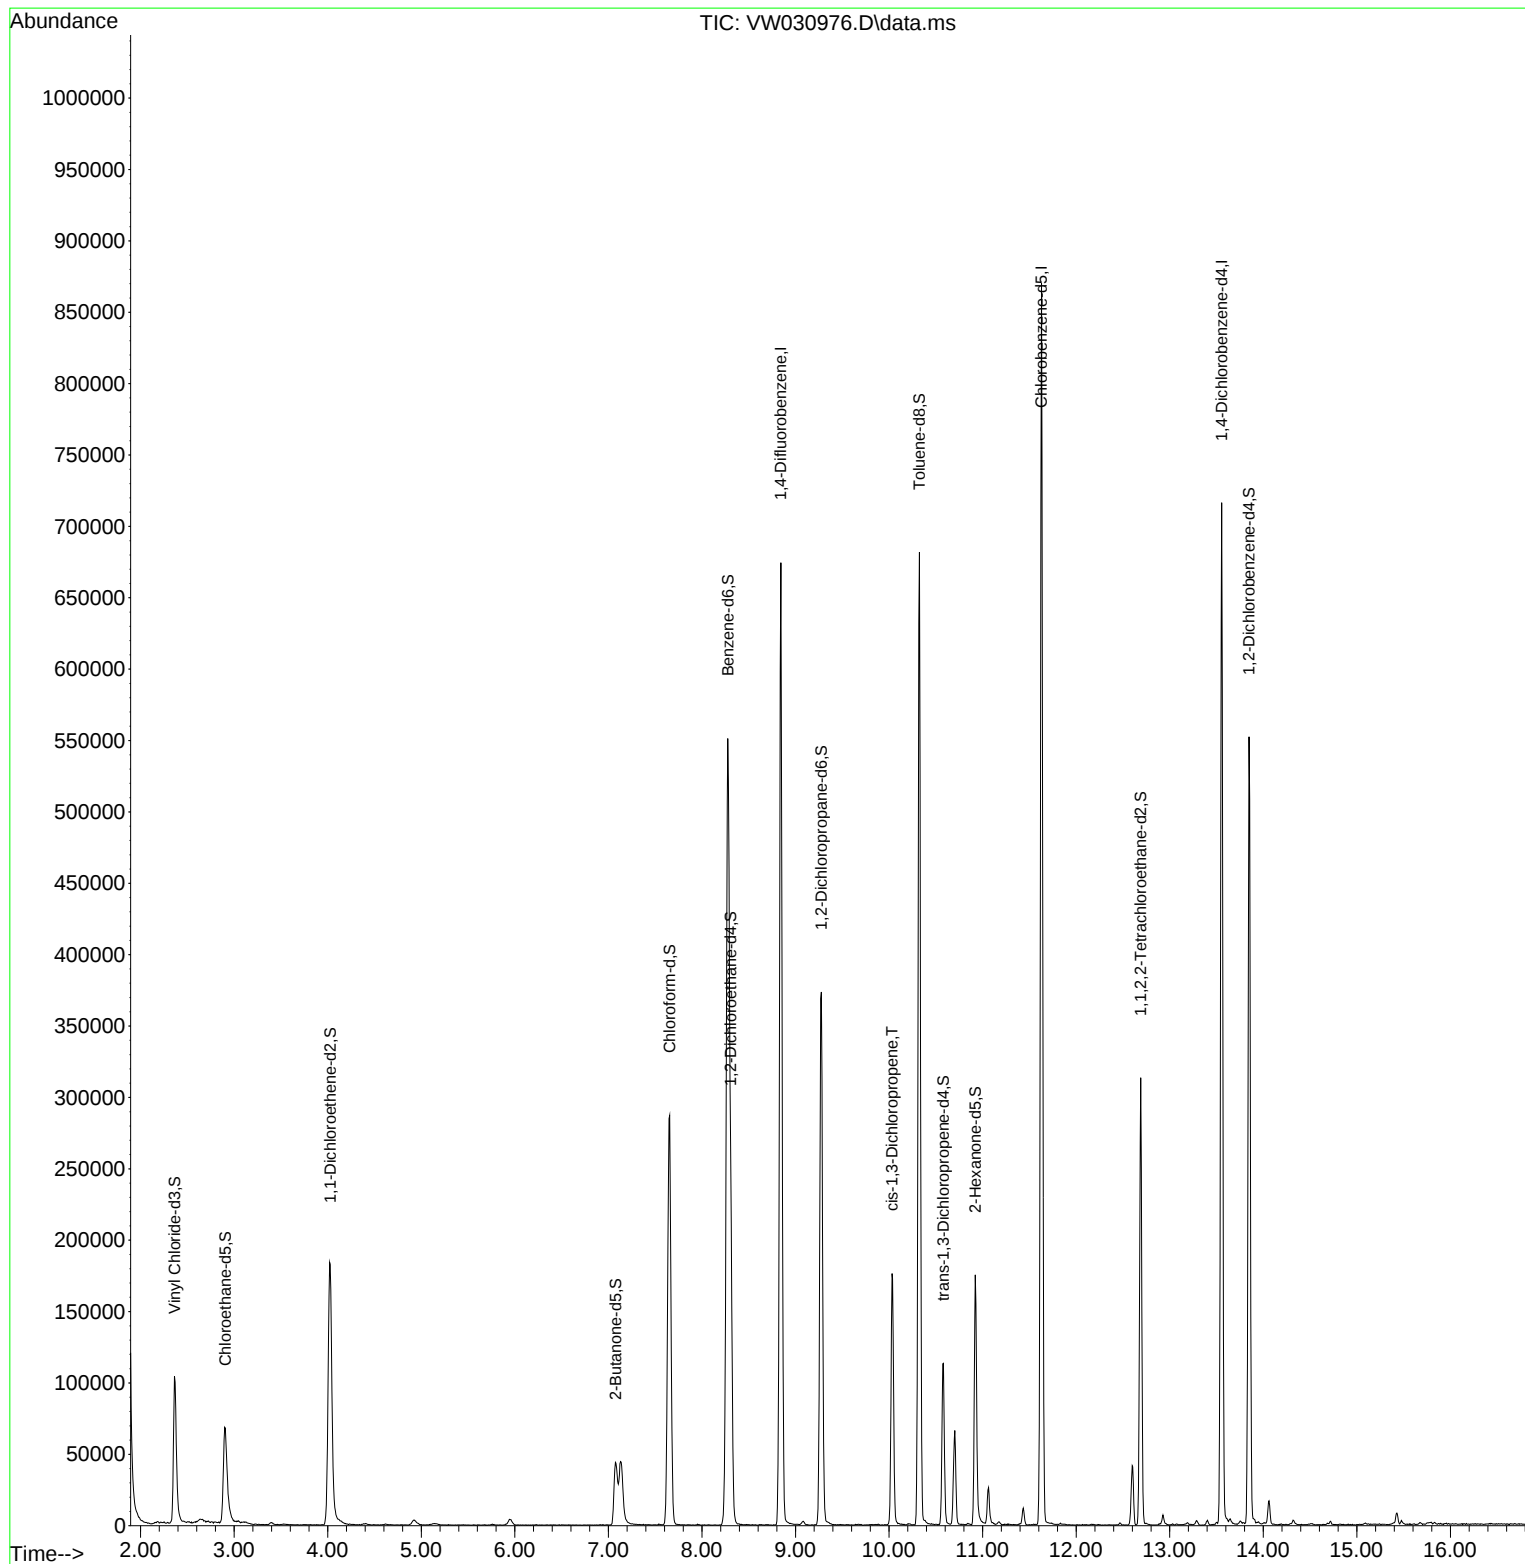

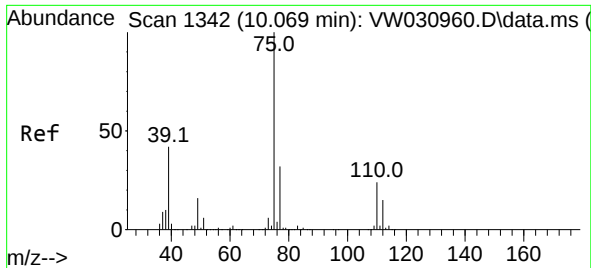

#39
cis-1,3-Dichloropropene
Concen: 0.389 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW030976.D
Acq: 08 Nov 2024 17:39

Instrument :
MSVOA_W
ClientSampleId :

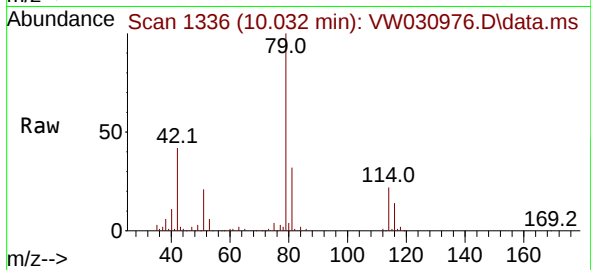

Tgt Ion: 75 Resp: 4450
Ion Ratio Lower Upper
75 100
77 62.6 21.3 39.6#

