

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
 Data File : VW030977.D
 Acq On : 08 Nov 2024 18:02
 Operator : SY/MD
 Sample : P4724-22
 Misc : 5.56g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 08 22:08:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Nov 08 22:04:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	600077	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	518112	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	214308	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	146372	14.872	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.480%
7) Chloroethane-d5	2.899	69	114385	15.154	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.600%
11) 1,1-Dichloroethene-d2	4.027	65	63518	15.641	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.560%
21) 2-Butanone-d5	7.081	46	79027	48.794	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.580%
24) Chloroform-d	7.648	84	327546	18.515	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.080%
26) 1,2-Dichloroethane-d4	8.307	65	172678	19.632	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.520%
32) Benzene-d6	8.276	84	609233	18.928	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.720%
36) 1,2-Dichloropropane-d6	9.276	67	196489	20.708	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.840%
41) Toluene-d8	10.319	98	491492	17.024	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.080%
43) trans-1,3-Dichloroprop...	10.575	79	72245	18.784	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.120%
47) 2-Hexanone-d5	10.922	63	62637	50.935	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.880%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	158451	23.968	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	156675	20.070	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.280%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	5099	0.408	ug/L	# 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
Data File : VW030977.D
Acq On : 08 Nov 2024 18:02
Operator : SY/MD
Sample : P4724-22
Misc : 5.56g/10mL/MSVOA_W/SOIL/A
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 08 22:08:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Nov 08 22:04:34 2024
Response via : Initial Calibration

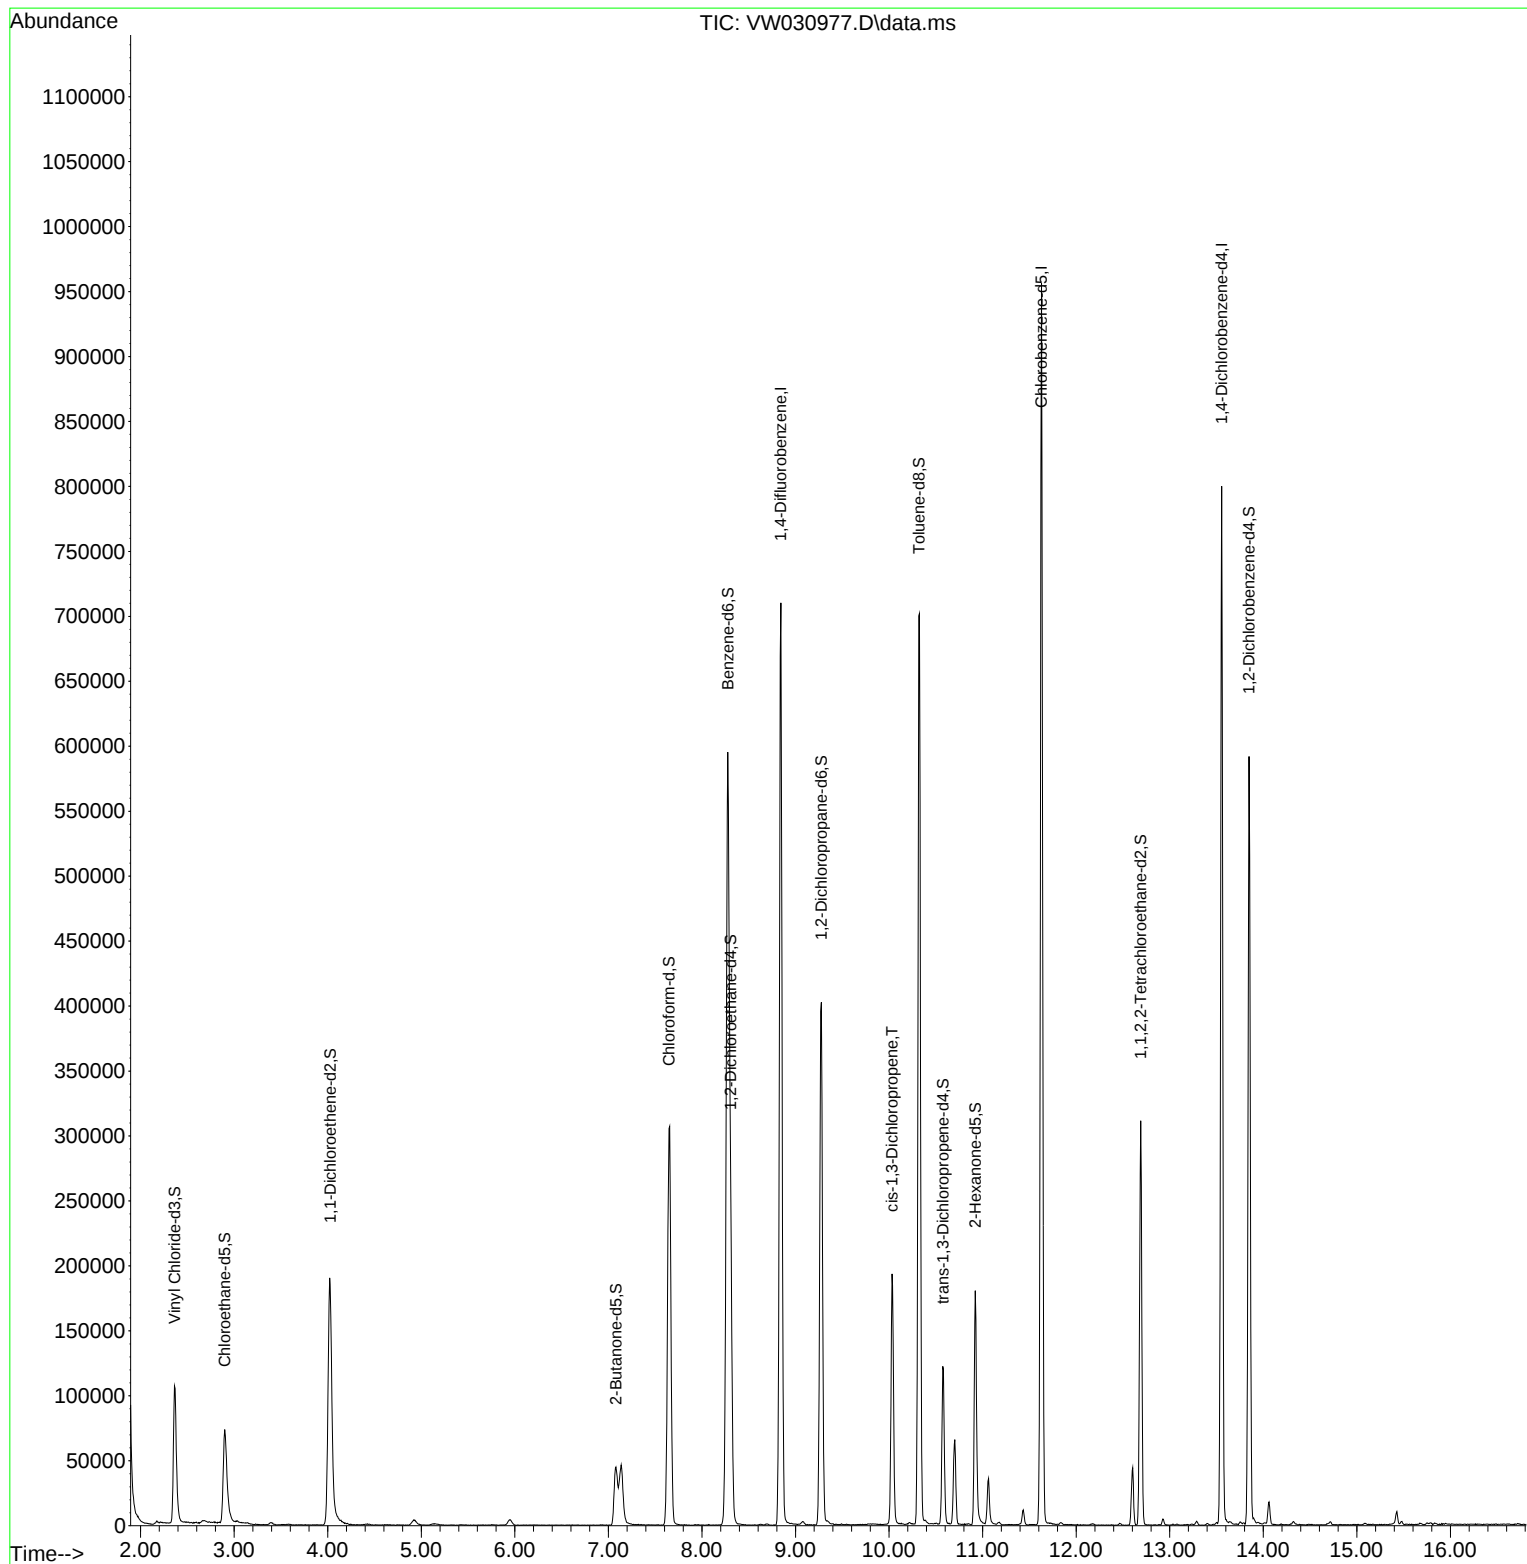

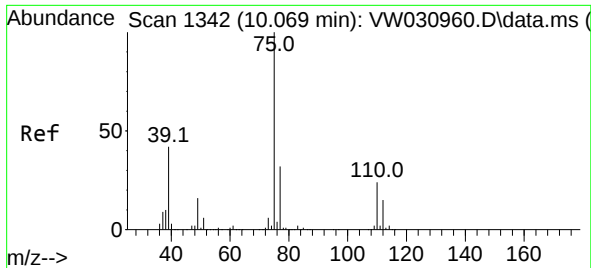

#39
 cis-1,3-Dichloropropene
 Concen: 0.408 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW030977.D
 Acq: 08 Nov 2024 18:02

Instrument :
 MSVOA_W
 ClientSampleId :

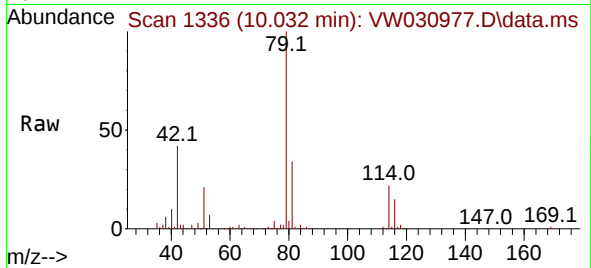

Tgt Ion: 75 Resp: 5099
 Ion Ratio Lower Upper
 75 100
 77 50.3 21.3 39.6#

