
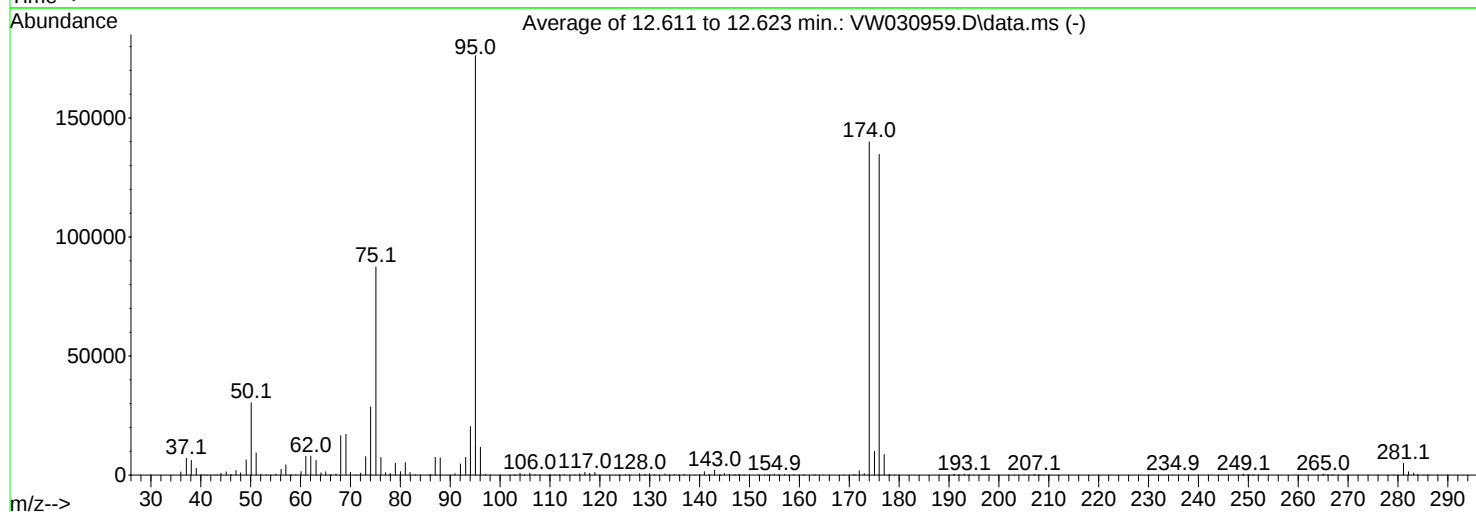


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW110824\
Data File : VW030959.D
Acq On : 08 Nov 2024 09:14
Operator : SY/MD
Sample : BFB594
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB594

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Tue Nov 12 00:19:56 2024

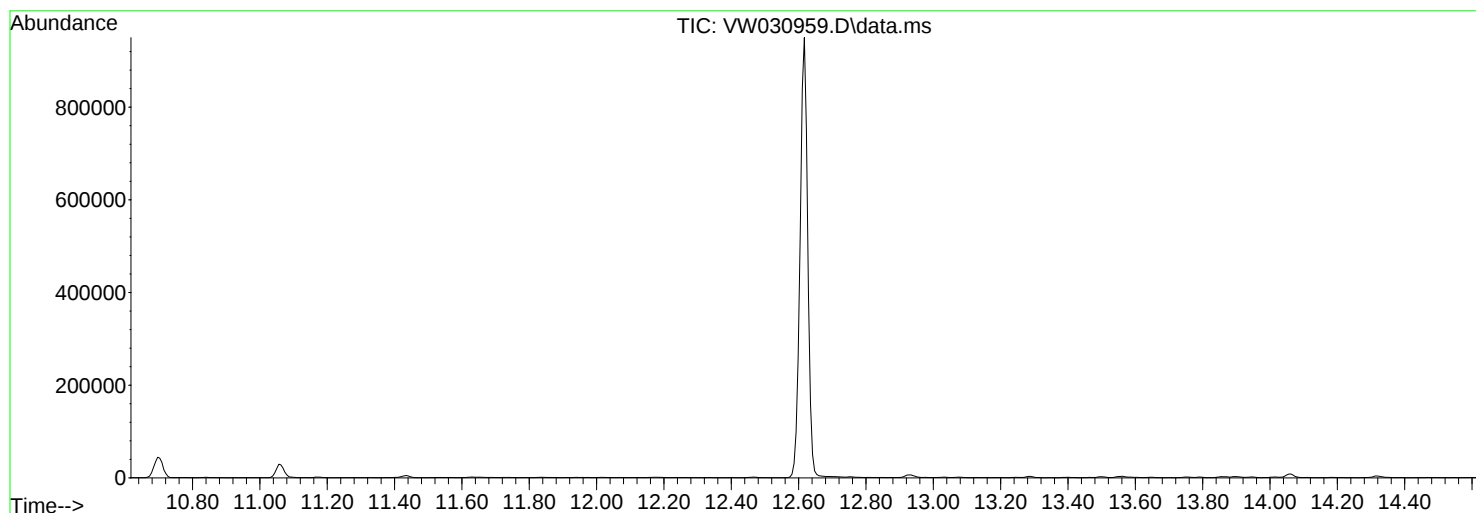

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	30360	PASS
75	95	30	80	49.6	87400	PASS
95	95	100	100	100.0	176149	PASS
96	95	5	9	6.6	11711	PASS
173	174	0.00	2	0.4	614	PASS
174	95	50	120	79.4	139923	PASS
175	174	5	9	7.1	9914	PASS
176	174	95	101	96.3	134696	PASS
177	176	5	9	6.4	8638	PASS

Scan 1751 (12.562 min): Vw030959.D\data.ms
BFB594

m/z	Abundance
39.90	226.0
44.20	222.0

Instrument :
MSVOA_W
ClientSampleId :
BFB594

m/z	Abundance
36.00	1527.0
37.10	7357.0
38.10	6953.0
39.10	2954.0
40.00	308.0
41.30	52.0
42.80	89.0
43.30	97.0
44.00	1179.0
45.10	1534.0
45.90	182.0
47.10	2103.0
48.00	892.0
49.10	6458.0
50.10	32344.0
51.10	10387.0
52.10	404.0
53.10	272.0
54.10	74.0
55.00	461.0
56.10	2421.0
57.00	4601.0
58.10	153.0
59.10	136.0
60.10	1654.0
61.00	8169.0
62.00	8831.0
63.10	6451.0
64.10	1113.0
65.10	1682.0
66.10	307.0
67.10	584.0
68.10	17144.0
69.10	18400.0
70.00	1155.0
71.10	80.0
72.10	901.0
73.10	8213.0
74.10	28448.0
75.10	89608.0
76.10	7720.0
77.10	989.0
77.90	645.0
79.00	5271.0
80.00	1579.0
81.00	5477.0
82.00	1122.0
83.00	127.0
86.20	292.0
87.00	7757.0
88.00	7351.0
91.00	657.0
92.00	4877.0
93.10	7702.0
94.10	20736.0
95.10	178944.0
96.10	12353.0
97.10	324.0
103.10	147.0
104.00	825.0
104.90	265.0
105.90	736.0
107.00	243.0
109.80	131.0
110.90	224.0
111.90	152.0
112.90	135.0
115.10	161.0
115.90	548.0
117.00	1147.0
118.00	742.0
119.00	1072.0
123.90	88.0
125.20	365.0
125.80	93.0
127.90	481.0
128.90	205.0
129.90	508.0
131.00	201.0
133.00	908.0
134.10	135.0
134.90	316.0
135.80	98.0
136.90	315.0
139.00	55.0
140.00	123.0
141.00	1324.0
141.80	129.0
143.00	2155.0
144.20	145.0
145.00	976.0
146.00	403.0

Instrument :
MSVOA_W
ClientSampleId :
BFB594

146.90	122.0
147.80	370.0
148.90	209.0
150.10	240.0
151.80	78.0
153.10	162.0
153.70	91.0
154.90	360.0
155.80	78.0
157.00	309.0
159.00	157.0
161.00	272.0
163.20	163.0
164.90	88.0
170.90	373.0
172.00	2118.0
173.00	1842.0
174.00	125240.0
175.10	9648.0
176.00	116664.0
177.00	7811.0
178.10	337.0
179.10	171.0
190.90	505.0
192.10	261.0
193.10	553.0
194.10	129.0
195.00	87.0
203.10	93.0
205.10	138.0
207.10	449.0
208.20	107.0
209.00	63.0
234.90	93.0
249.00	700.0
249.90	94.0
250.30	79.0
250.90	164.0
251.20	171.0
252.10	60.0
265.00	968.0
266.00	266.0
266.80	244.0
279.10	93.0
281.10	7258.0
282.20	2089.0
283.10	1403.0
283.90	350.0
285.20	171.0
286.00	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB594

m/z	Abundance
36.00	1386.0
37.10	7890.0
38.10	6777.0
39.10	3187.0
40.20	362.0
40.80	107.0
42.90	118.0
43.30	126.0
44.10	913.0
45.10	1405.0
46.20	270.0
47.00	2113.0
47.90	1093.0
49.10	7550.0
50.10	34240.0
51.10	10442.0
52.00	387.0
53.10	178.0
54.10	81.0
55.10	458.0
56.10	2666.0
57.10	4789.0
58.10	294.0
60.10	1657.0
61.00	9662.0
62.10	8679.0
63.10	6929.0
64.10	1030.0
65.00	1432.0
66.20	120.0
67.00	412.0
68.10	18408.0
69.10	18864.0
70.00	1294.0
71.10	91.0
72.00	894.0
73.10	8606.0
74.00	32808.0
75.10	98240.0
76.10	8376.0
77.10	1343.0
78.00	862.0
79.00	5704.0
80.00	1527.0
81.00	5935.0
81.90	1100.0
83.00	205.0
84.10	55.0
86.10	317.0
87.00	8999.0
88.00	7973.0
90.90	594.0
92.10	5085.0
93.10	8437.0
94.10	22832.0
95.00	199104.0
96.00	13082.0
97.10	468.0
102.80	78.0
104.00	798.0
104.90	235.0
105.90	747.0
107.00	265.0
108.00	54.0
110.10	215.0
111.00	167.0
111.90	114.0
112.90	155.0
115.10	110.0
115.90	566.0
117.00	1358.0
117.90	755.0
119.00	1170.0
123.20	64.0
123.80	57.0
125.00	175.0
125.90	77.0
128.00	624.0
129.10	369.0
129.90	665.0
130.90	296.0
133.10	355.0
134.00	144.0
135.00	429.0
135.80	68.0
136.90	249.0
140.10	120.0
141.00	1562.0
142.10	295.0
143.00	2430.0
143.90	145.0
144.90	673.0

Instrument :
MSVOA_W
ClientSampleId :
BFB594

145.80	384.0
147.30	168.0
148.10	453.0
148.90	180.0
149.90	190.0
151.90	97.0
153.00	149.0
153.70	85.0
154.20	116.0
155.00	501.0
155.80	81.0
157.10	314.0
158.90	309.0
161.00	196.0
162.90	107.0
169.00	72.0
171.10	414.0
172.00	2019.0
174.00	152832.0
175.00	10869.0
176.00	155584.0
177.00	10097.0
178.00	273.0
179.10	110.0
191.10	429.0
191.90	71.0
193.00	527.0
193.80	81.0
205.00	83.0
207.10	293.0
207.90	66.0
249.10	353.0
250.10	87.0
250.40	87.0
251.10	98.0
265.00	335.0
265.90	139.0
267.10	90.0
279.20	57.0
281.10	5352.0
282.00	1513.0
283.20	893.0
283.90	271.0

Instrument :
MSVOA_W
ClientSampleId :
BFB594

m/z	Abundance
36.00	984.0
37.10	5672.0
38.10	4971.0
39.10	2361.0
40.00	299.0
40.80	73.0
44.00	766.0
45.10	1086.0
46.00	107.0
47.00	1463.0
48.00	729.0
49.10	5241.0
50.10	24496.0
51.10	7101.0
52.00	388.0
52.90	53.0
55.10	421.0
56.10	2191.0
57.00	3540.0
58.10	157.0
58.90	80.0
60.00	1096.0
61.10	5945.0
62.00	6336.0
63.10	5095.0
64.10	725.0
65.00	1026.0
65.90	61.0
66.30	62.0
67.20	369.0
68.00	14140.0
69.10	14118.0
70.00	1001.0
72.10	731.0
73.00	6569.0
74.10	24704.0
75.10	74352.0
76.10	6048.0
77.00	812.0
78.00	695.0
79.00	3938.0
80.10	1199.0
81.00	4274.0
82.00	965.0
83.00	112.0
85.80	274.0
87.00	5662.0
88.00	6385.0
91.00	612.0
92.10	4031.0
93.10	6322.0
94.00	17528.0
95.10	150400.0
96.10	9698.0
97.20	207.0
102.90	59.0
104.00	668.0
104.90	219.0
106.00	628.0
106.90	164.0
110.20	56.0
111.10	83.0
111.90	90.0
112.90	128.0
114.90	193.0
116.00	428.0
117.00	989.0
118.00	711.0
119.00	1032.0
123.90	118.0
125.00	75.0
125.90	108.0
128.00	581.0
129.10	419.0
130.00	509.0
131.00	209.0
132.90	218.0
133.70	83.0
135.00	341.0
136.90	216.0
140.00	149.0
140.90	1402.0
142.00	173.0
143.00	1664.0
144.00	154.0
145.00	391.0
146.00	315.0
147.10	121.0
147.70	265.0
149.00	105.0
149.80	136.0
150.10	152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB594

151.90	63.0
153.00	151.0
154.20	66.0
154.90	462.0
156.00	127.0
157.00	279.0
157.90	65.0
158.80	184.0
160.80	270.0
168.90	61.0
170.90	148.0
172.00	1464.0
174.00	141696.0
175.00	9226.0
176.00	131840.0
177.00	8006.0
178.00	279.0
191.10	124.0
193.00	153.0
207.00	182.0
248.80	100.0
249.20	109.0
265.20	159.0
281.10	2164.0
282.20	595.0
283.10	382.0

Instrument :
MSVOA_W
ClientSampleId :
BFB594