
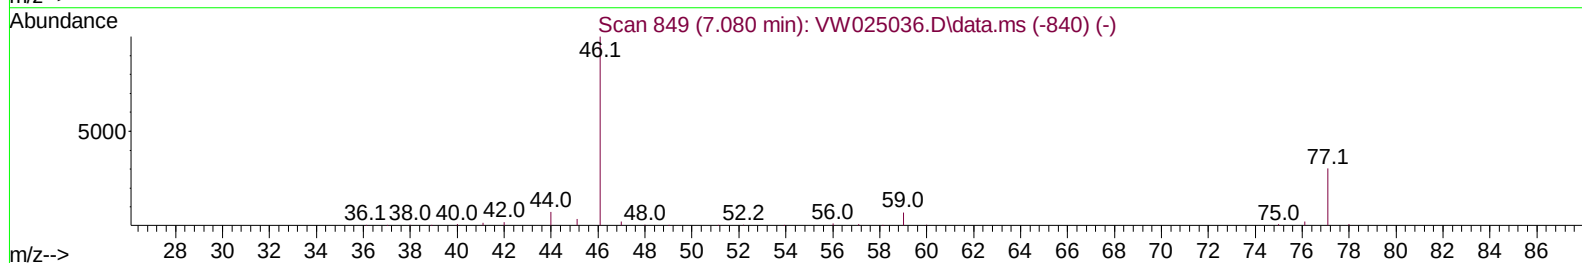
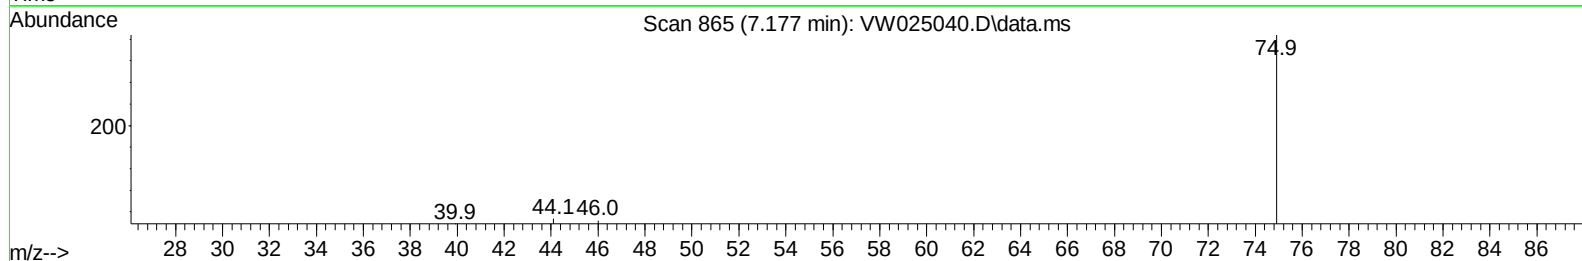


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
Data File : VW025040.D
Acq On : 11 Nov 2022 17:21
Operator : SY/VA
Sample : N5603-05
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 00:49:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 12 00:48:53 2022
Response via : Initial Calibration

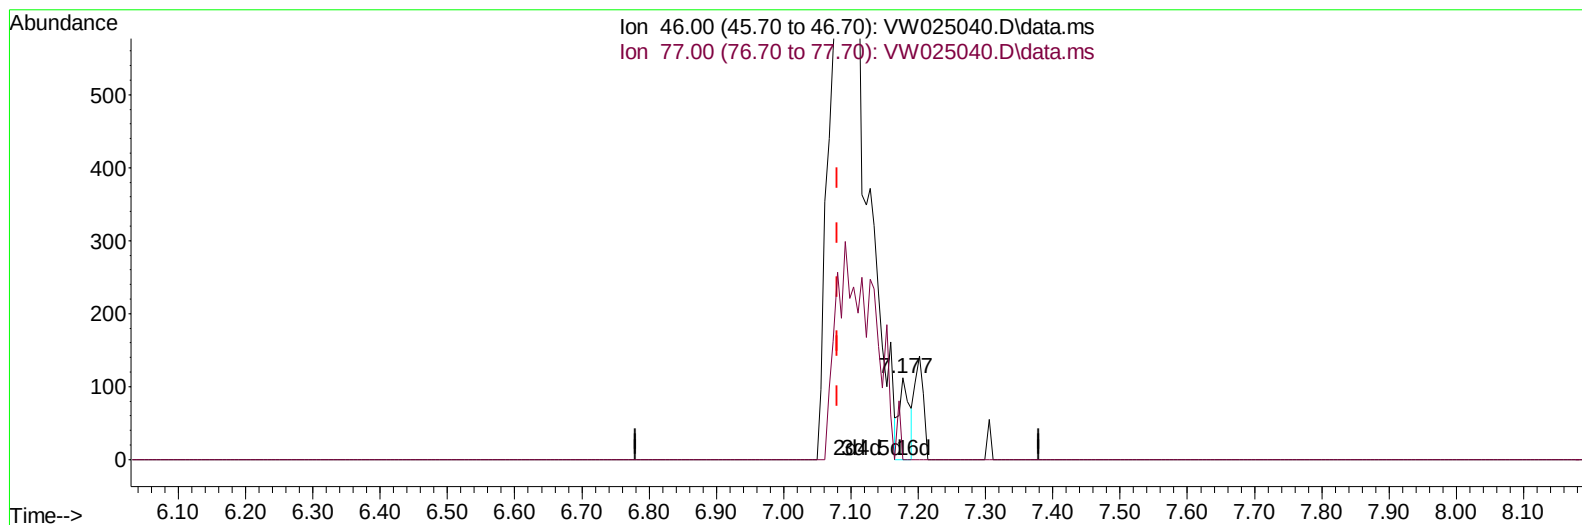

TIC: VW025040.D\data.ms

(21) 2-Butanone-d5 (S)




7.177min (+ 0.098) 1.34 ug/L

response 118

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.30	25.42
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
Data File : VW025040.D
Acq On : 11 Nov 2022 17:21
Operator : SY/VA
Sample : N5603-05
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 00:49:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 12 00:48:53 2022
Response via : Initial Calibration

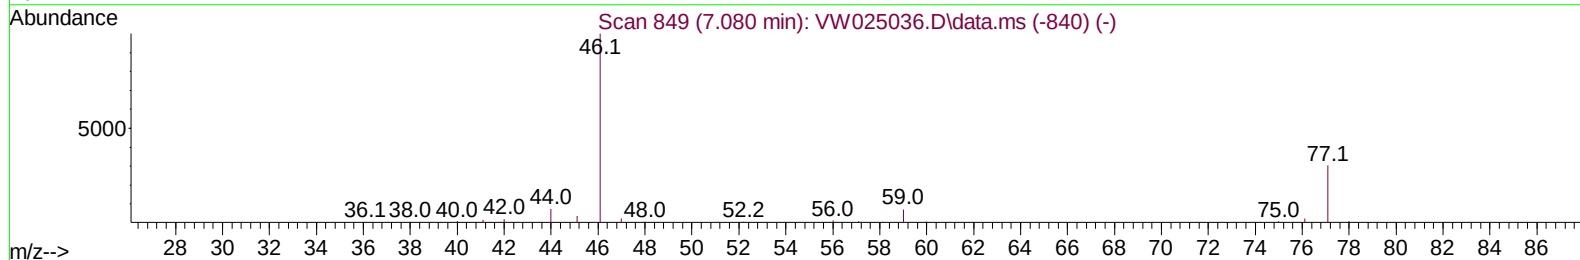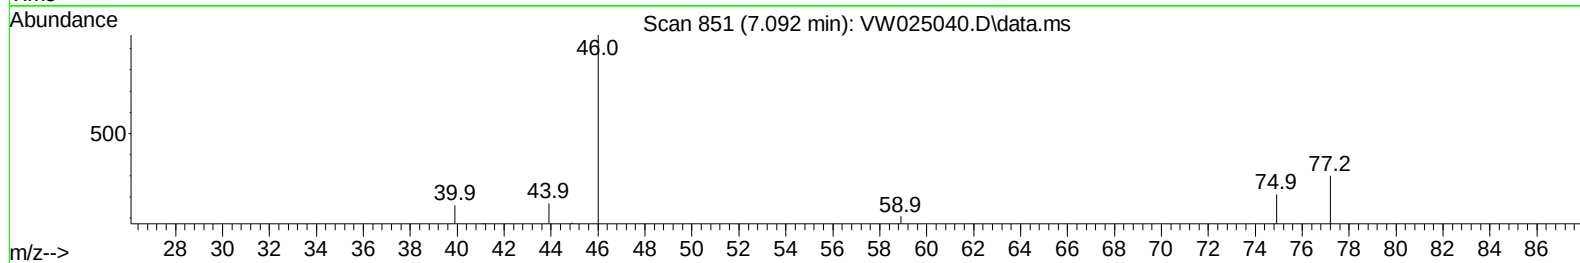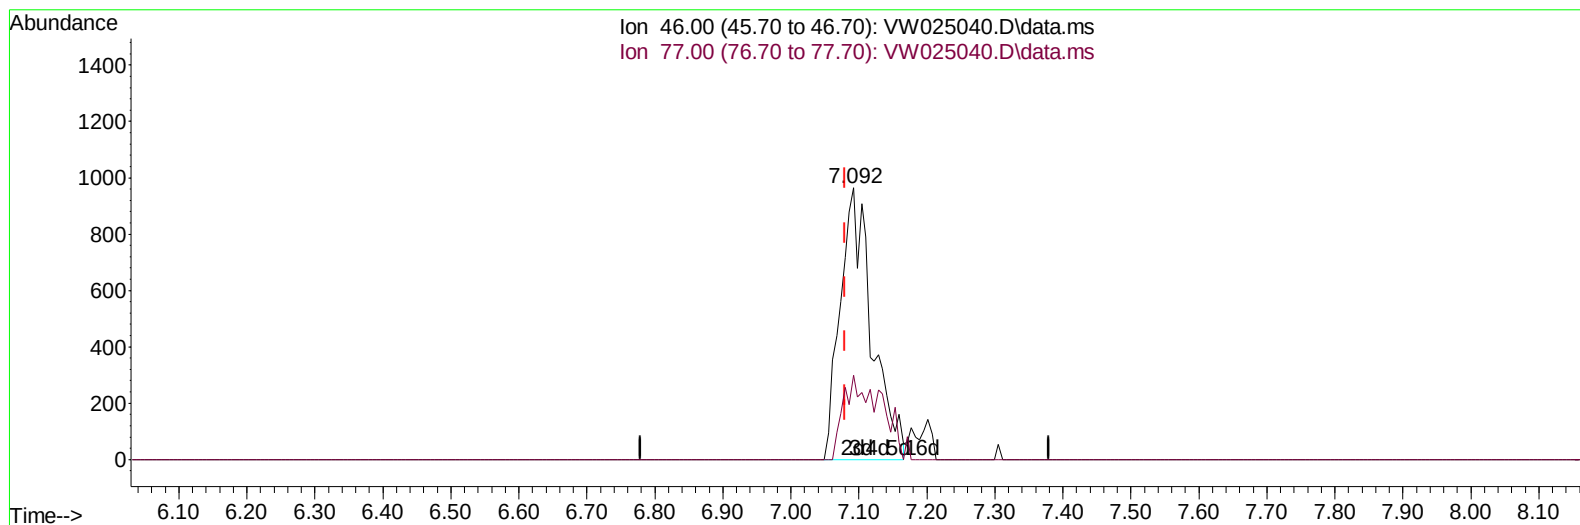

TIC: VW025040.D\data.ms

(21) 2-Butanone-d5 (S)




7.092min (+ 0.012) 35.17 ug/L m

response 3107

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	27.30	0.97#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
Data File : VW025040.D
Acq On : 11 Nov 2022 17:21
Operator : SY/VA
Sample : N5603-05
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 00:49:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 12 00:48:53 2022
Response via : Initial Calibration

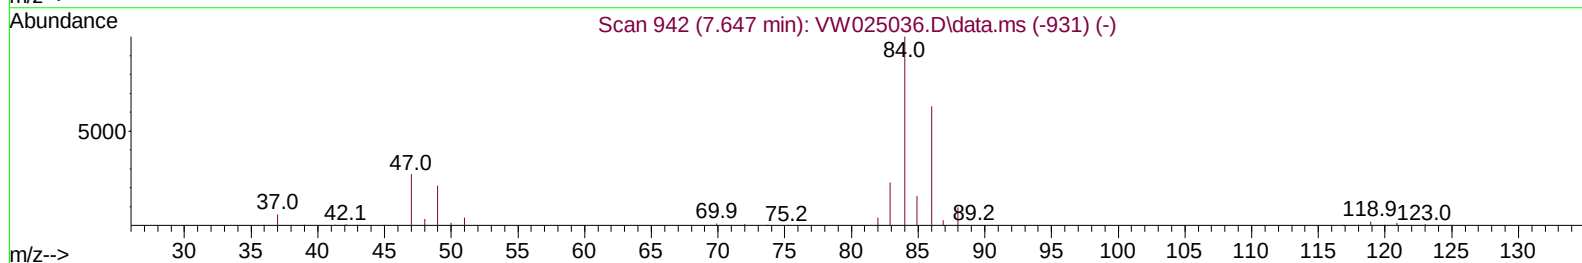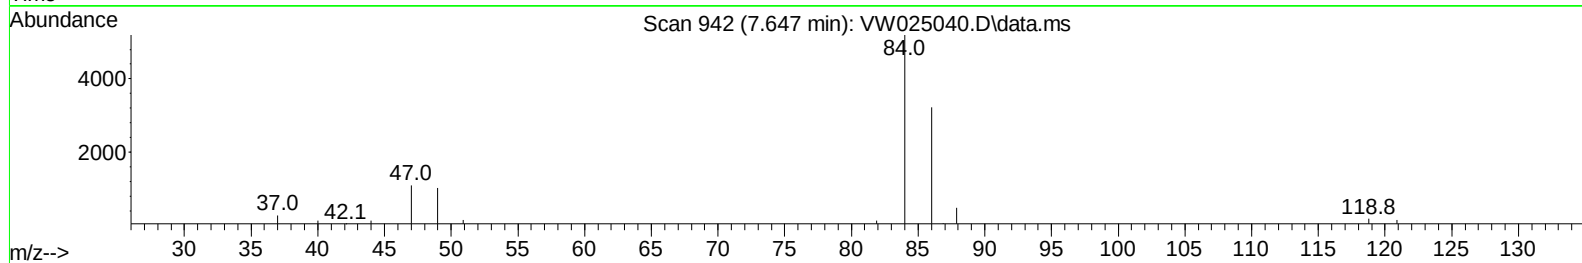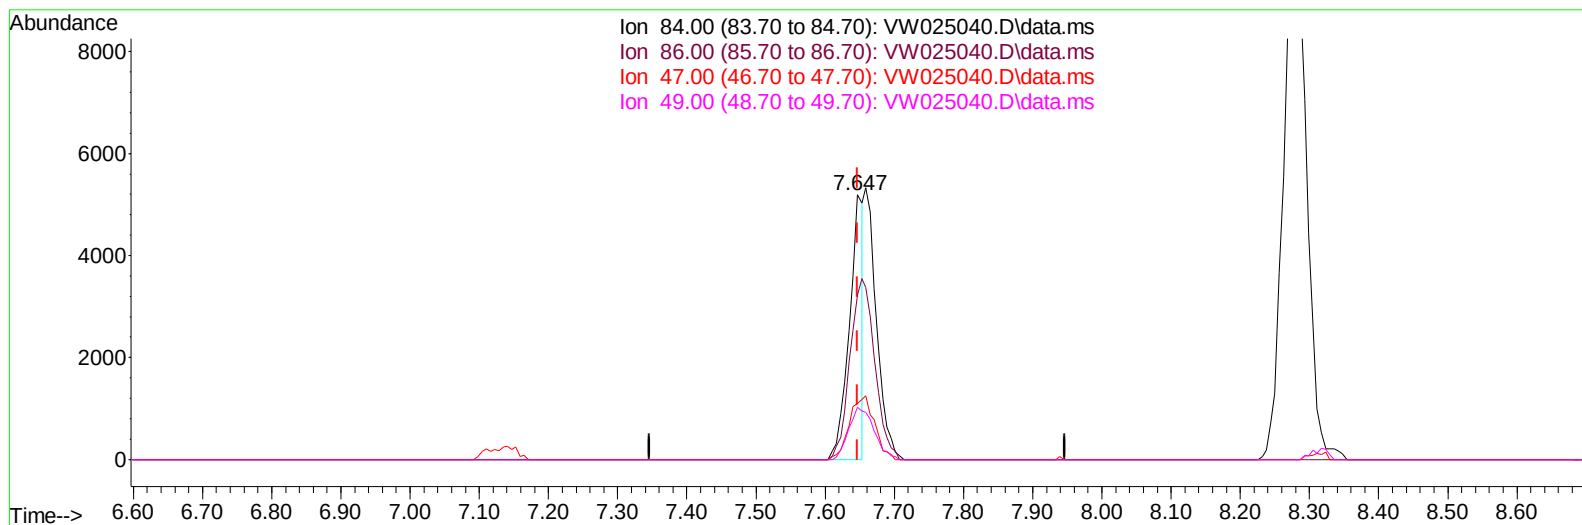

TIC: VW025040.D\data.ms

(24) Chloroform-d (S)




7.647min (+ 0.000) 9.94 ug/L

response 7037

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.30	124.39#
47.00	39.70	44.27
49.00	24.60	36.86#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
Data File : VW025040.D
Acq On : 11 Nov 2022 17:21
Operator : SY/VA
Sample : N5603-05
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 00:49:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 12 00:48:53 2022
Response via : Initial Calibration

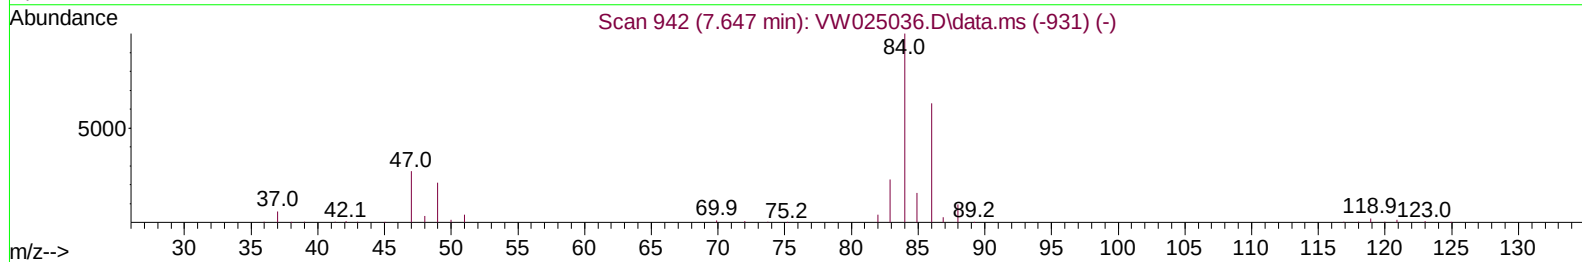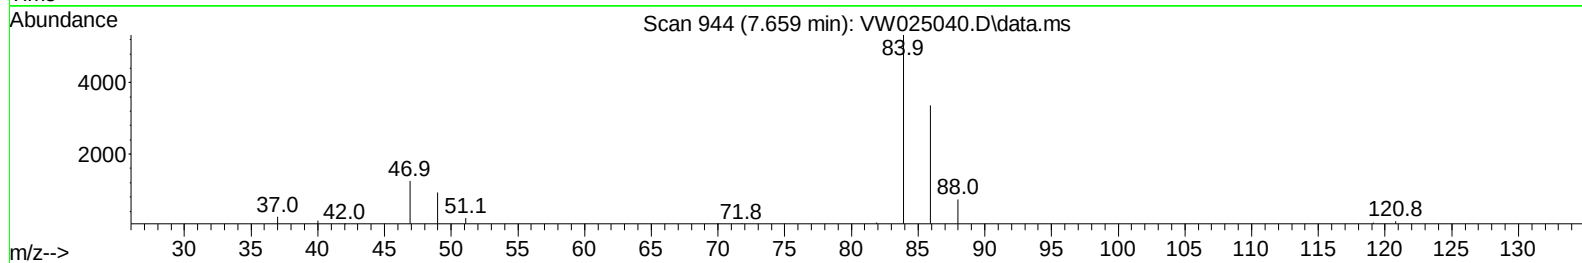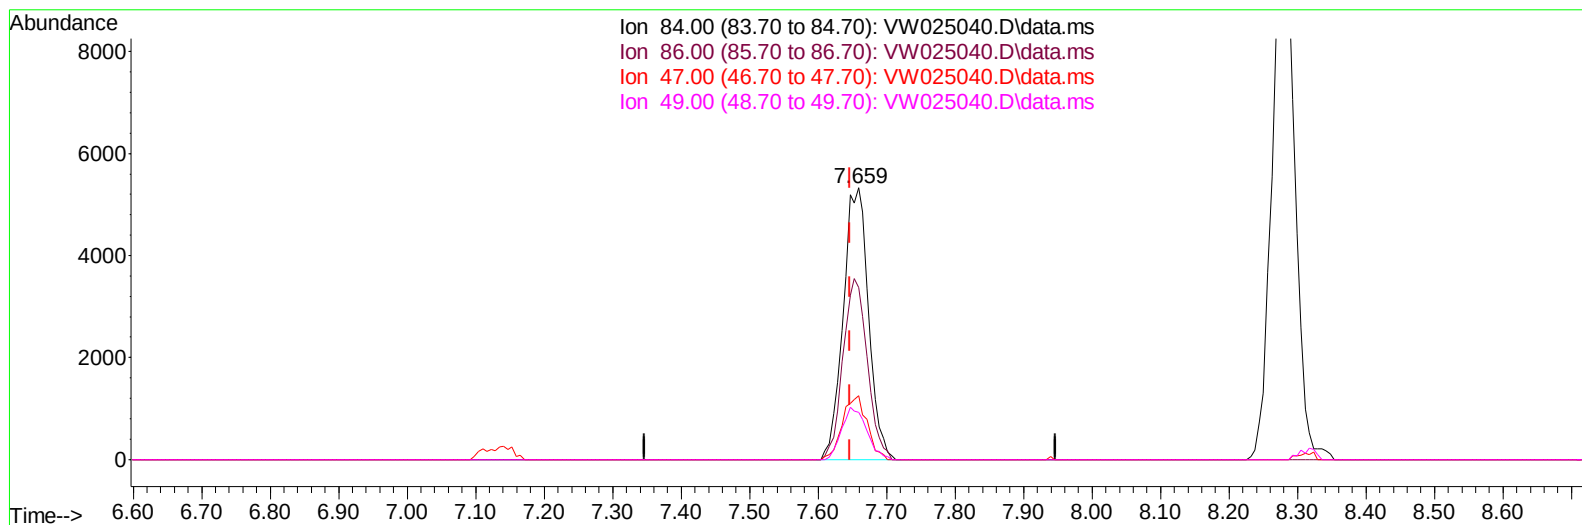

TIC: VW025040.D\data.ms

(24) Chloroform-d (S)

7.659min (+ 0.012) 19.32 ug/L m

response 13674

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.30	64.01
47.00	39.70	22.78#
49.00	24.60	18.97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw111122\
 Data File : VW025040.D
 Acq On : 11 Nov 2022 17:21
 Operator : SY/VA
 Sample : N5603-05
 Misc : 5.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 00:49:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 12 00:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	23319	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	22603	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	8057	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	3371	12.879	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	51.520%	
7) Chloroethane-d5	2.891	69	4585	29.904	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	119.600%	
11) 1,1-Dichloroethene-d2	4.031	63	7760	11.902	ug/L	0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	47.600%	
21) 2-Butanone-d5	7.092	46	3107m	35.172	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	70.340%	
24) Chloroform-d	7.659	84	13674m	19.322	ug/L	0.01
Spiked Amount 25.000	Range 40	- 150	Recovery	=	77.280%	
26) 1,2-Dichloroethane-d4	8.311	65	8288	20.922	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	83.680%	
32) Benzene-d6	8.281	84	24316	16.784	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	67.120%	
36) 1,2-Dichloropropane-d6	9.281	67	7274	17.136	ug/L	0.01
Spiked Amount 25.000	Range 70	- 120	Recovery	=	68.560%#	
41) Toluene-d8	10.323	98	20733	15.372	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	61.480%	
43) trans-1,3-Dichloroprop...	10.585	79	2996	15.917	ug/L	0.01
Spiked Amount 25.000	Range 30	- 135	Recovery	=	63.680%	
47) 2-Hexanone-d5	10.927	63	1746	23.811	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	47.620%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	5842	17.236	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	68.960%	
66) 1,2-Dichlorobenzene-d4	13.853	152	5943	19.194	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	76.760%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
Data File : VW025040.D
Acq On : 11 Nov 2022 17:21
Operator : SY/VA
Sample : N5603-05
Misc : 5.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 00:49:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 12 00:48:53 2022
Response via : Initial Calibration

