

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
 Data File : VW025039.D
 Acq On : 11 Nov 2022 16:57
 Operator : SY/VA
 Sample : VIBLK581
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK581

Quant Time: Nov 12 00:49:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 12 00:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	293324	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	263211	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	128632	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	50710	15.402	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	61.600%		
7) Chloroethane-d5	2.891	69	32237	16.715	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.840%		
11) 1,1-Dichloroethene-d2	4.019	63	114580	13.971	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	55.880%		
21) 2-Butanone-d5	7.074	46	44268	39.839	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.680%		
24) Chloroform-d	7.653	84	190421	21.391	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.560%		
26) 1,2-Dichloroethane-d4	8.305	65	109463m	21.967	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	87.880%		
32) Benzene-d6	8.275	84	363536	21.548	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.200%		
36) 1,2-Dichloropropane-d6	9.274	67	103501	20.938	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	83.760%		
41) Toluene-d8	10.323	98	327413	20.846	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	83.400%		
43) trans-1,3-Dichloroprop...	10.579	79	44980	20.521	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.080%		
47) 2-Hexanone-d5	10.927	63	35153	41.167	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	82.340%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	80484	20.391	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	81.560%		
66) 1,2-Dichlorobenzene-d4	13.853	152	107284	21.703	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	86.800%		
Target Compounds						Qvalue
16) Methylene chloride	4.922	84	21240	4.078	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
Data File : VW025039.D
Acq On : 11 Nov 2022 16:57
Operator : SY/VA
Sample : VIBLK581
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK581

Quant Time: Nov 12 00:49:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 12 00:48:53 2022
Response via : Initial Calibration

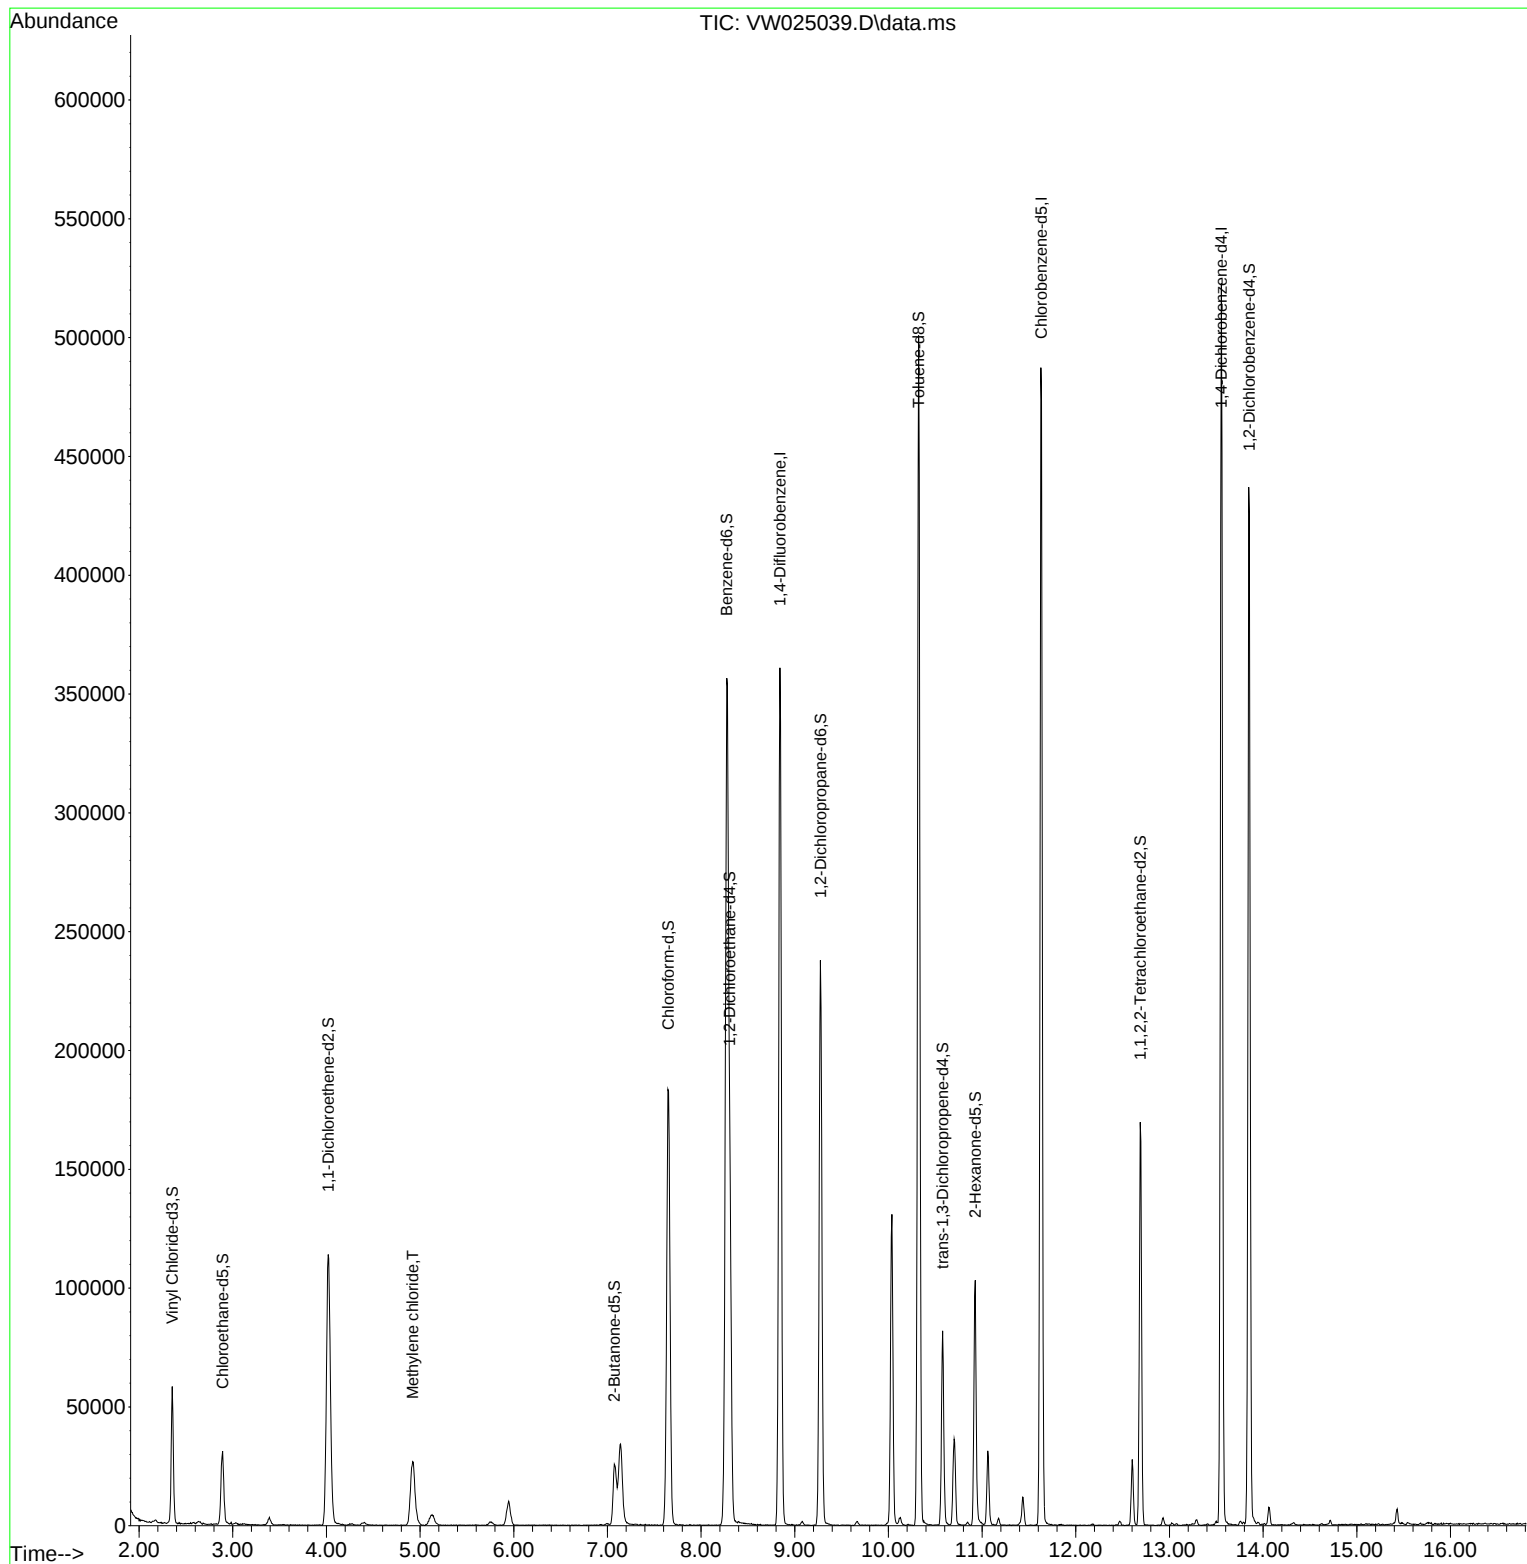

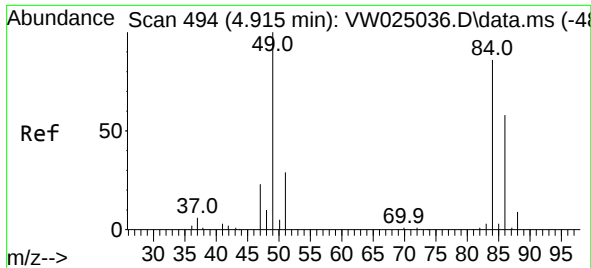

#16
Methylene chloride
Concen: 4.078 ug/L
RT: 4.922 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW025039.D
Acq: 11 Nov 2022 16:57

Instrument :
MSVOA_W
ClientSampleId :
VIBLK581

Tgt Ion: 84 Resp: 21240
Ion Ratio Lower Upper
84 100
86 65.6 42.6 79.0
49 124.9 81.9 152.1

