

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
 Data File : VW025041.D
 Acq On : 11 Nov 2022 17:45
 Operator : SY/VA
 Sample : VIBLK582
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK582

Quant Time: Nov 12 00:50:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 12 00:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	281099	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	260449	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	123776	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	52839	16.747	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.000%
7) Chloroethane-d5	2.885	69	33172	17.948	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.800%
11) 1,1-Dichloroethene-d2	4.019	63	121598	15.472	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.880%
21) 2-Butanone-d5	7.074	46	48561	45.603	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.200%
24) Chloroform-d	7.647	84	202153	23.697	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	8.305	65	117311	24.566	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.280%
32) Benzene-d6	8.275	84	388064	23.246	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.000%
36) 1,2-Dichloropropane-d6	9.274	67	111184	22.731	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.920%
41) Toluene-d8	10.323	98	353052	22.716	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.880%
43) trans-1,3-Dichloroprop...	10.579	79	47953	22.109	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.440%
47) 2-Hexanone-d5	10.920	63	38443	45.497	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.000%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	90584	23.193	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	115346	24.249	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.000%
Target Compounds						Qvalue
16) Methylene chloride	4.922	84	21368	4.281	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111122\
Data File : VW025041.D
Acq On : 11 Nov 2022 17:45
Operator : SY/VA
Sample : VIBLK582
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK582

Quant Time: Nov 12 00:50:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 12 00:48:53 2022
Response via : Initial Calibration

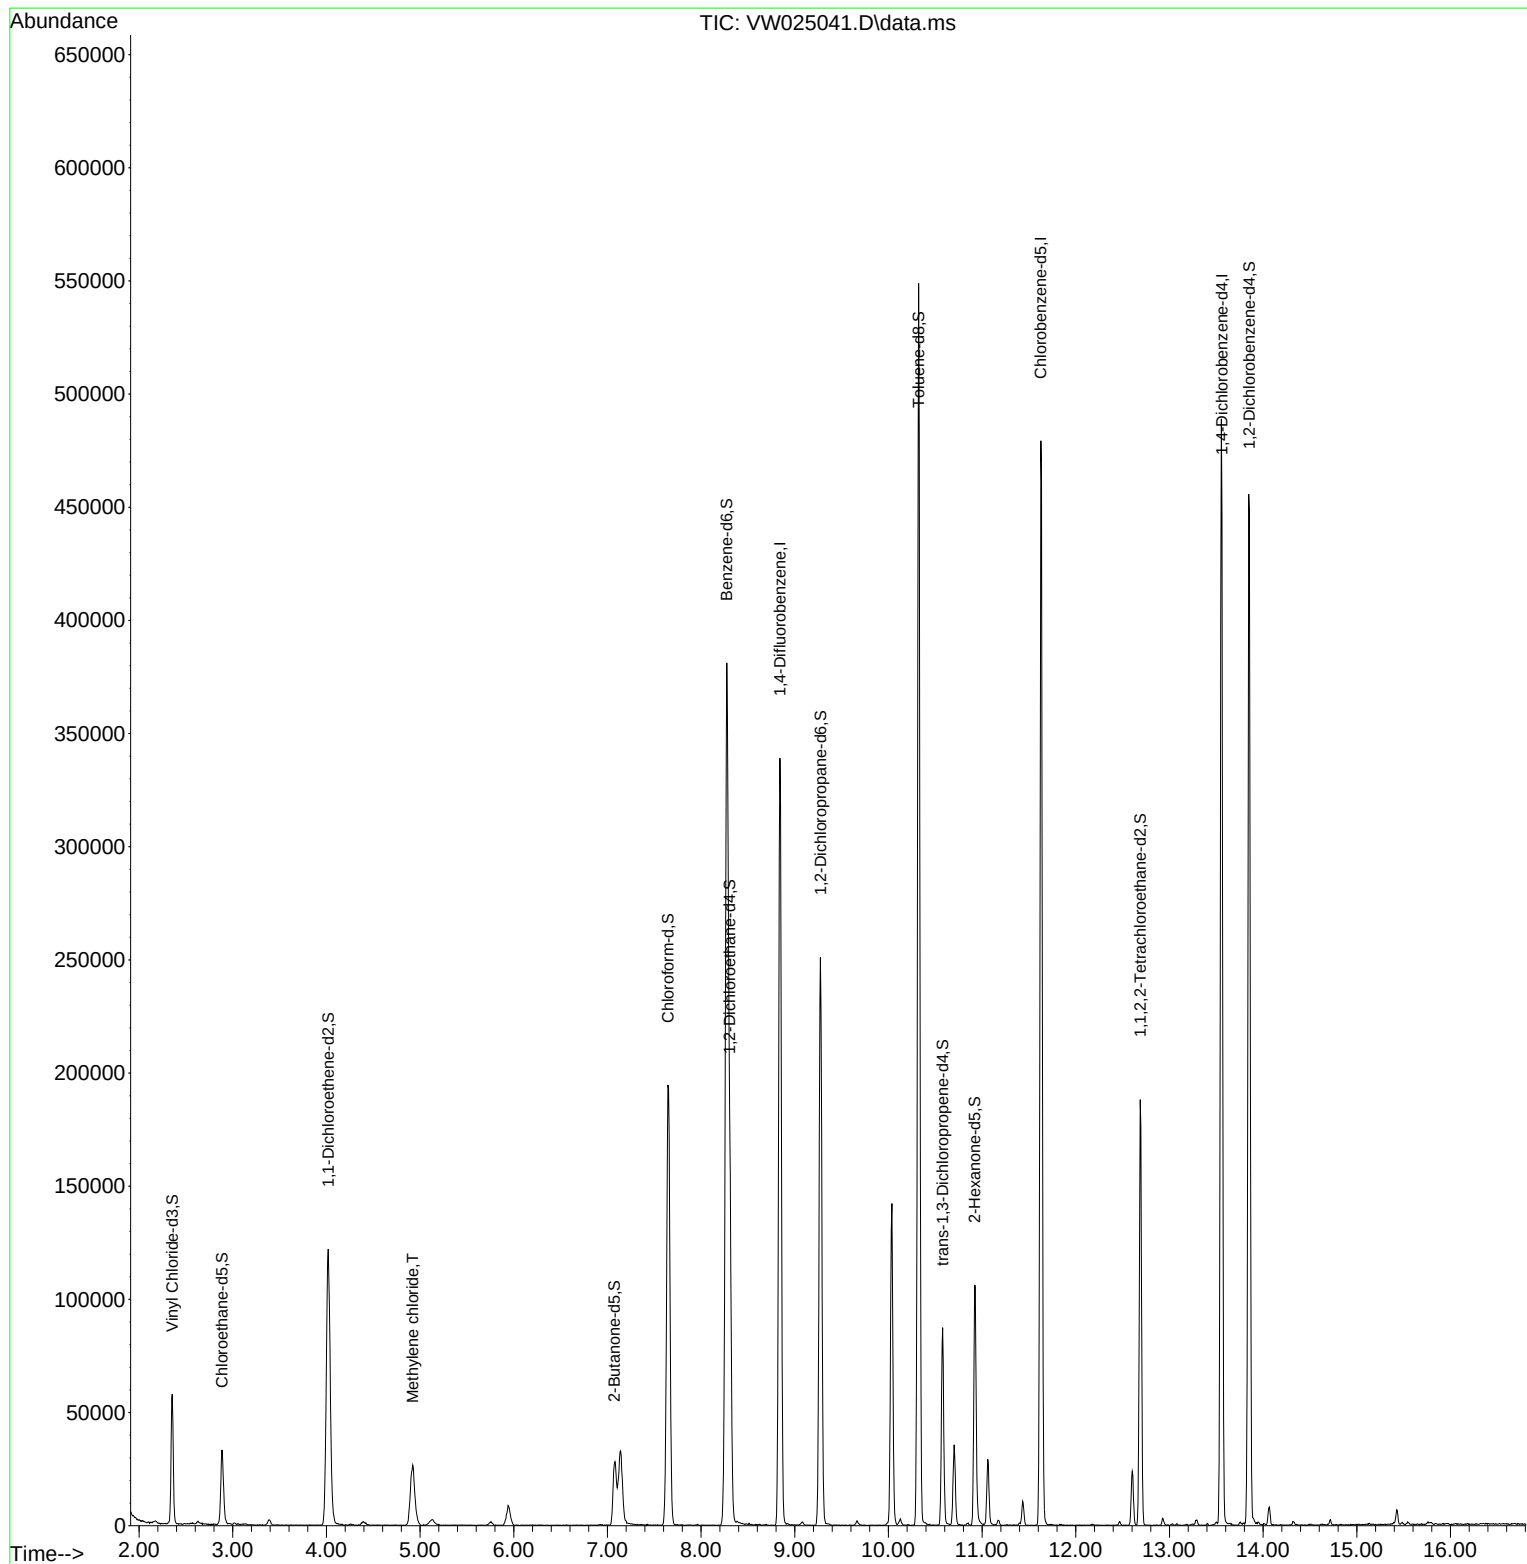

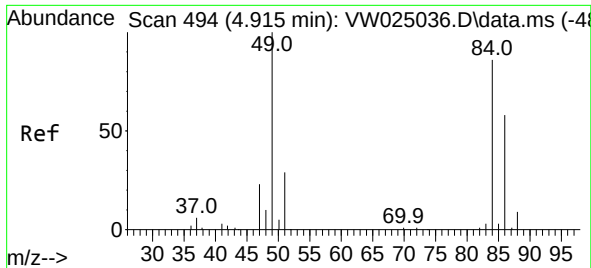

#16

Methylene chloride

Concen: 4.281 ug/L

RT: 4.922 min Scan# 49

Delta R.T. 0.006 min

Lab File: VW025041.D

Acq: 11 Nov 2022 17:45

Instrument :

MSVOA_W

ClientSampleId :

VIBLK582

Tgt Ion: 84 Resp: 21368

Ion Ratio Lower Upper

84 100

86 61.2 42.6 79.0

49 115.5 81.9 152.1

