

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111124\
 Data File : VW030983.D
 Acq On : 11 Nov 2024 10:40
 Operator : SY/MD
 Sample : VW1111SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 12 00:20:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 12 00:19:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	447704	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	436679	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	185286	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	93342	12.712	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	50.840%		
7) Chloroethane-d5	2.899	69	77385	13.741	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	54.960%		
11) 1,1-Dichloroethene-d2	4.021	65	44788	14.782	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	59.120%		
21) 2-Butanone-d5	7.075	46	49577	41.028	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	82.060%		
24) Chloroform-d	7.648	84	244877	18.554	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	74.200%		
26) 1,2-Dichloroethane-d4	8.307	65	124614	18.989	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	75.960%		
32) Benzene-d6	8.276	84	470572	17.346	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	69.400%		
36) 1,2-Dichloropropane-d6	9.276	67	144953	18.125	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	72.520%		
41) Toluene-d8	10.318	98	413543	16.995	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	67.960%		
43) trans-1,3-Dichloroprop...	10.574	79	54273	16.742	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	66.960%		
47) 2-Hexanone-d5	10.922	63	41112	39.666	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.340%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	113094	20.298	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	81.200%		
66) 1,2-Dichlorobenzene-d4	13.848	152	138959	20.589	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.360%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3739	0.355	ug/L	# 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111124\
Data File : VW030983.D
Acq On : 11 Nov 2024 10:40
Operator : SY/MD
Sample : VW1111SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 12 00:20:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 12 00:19:56 2024
Response via : Initial Calibration

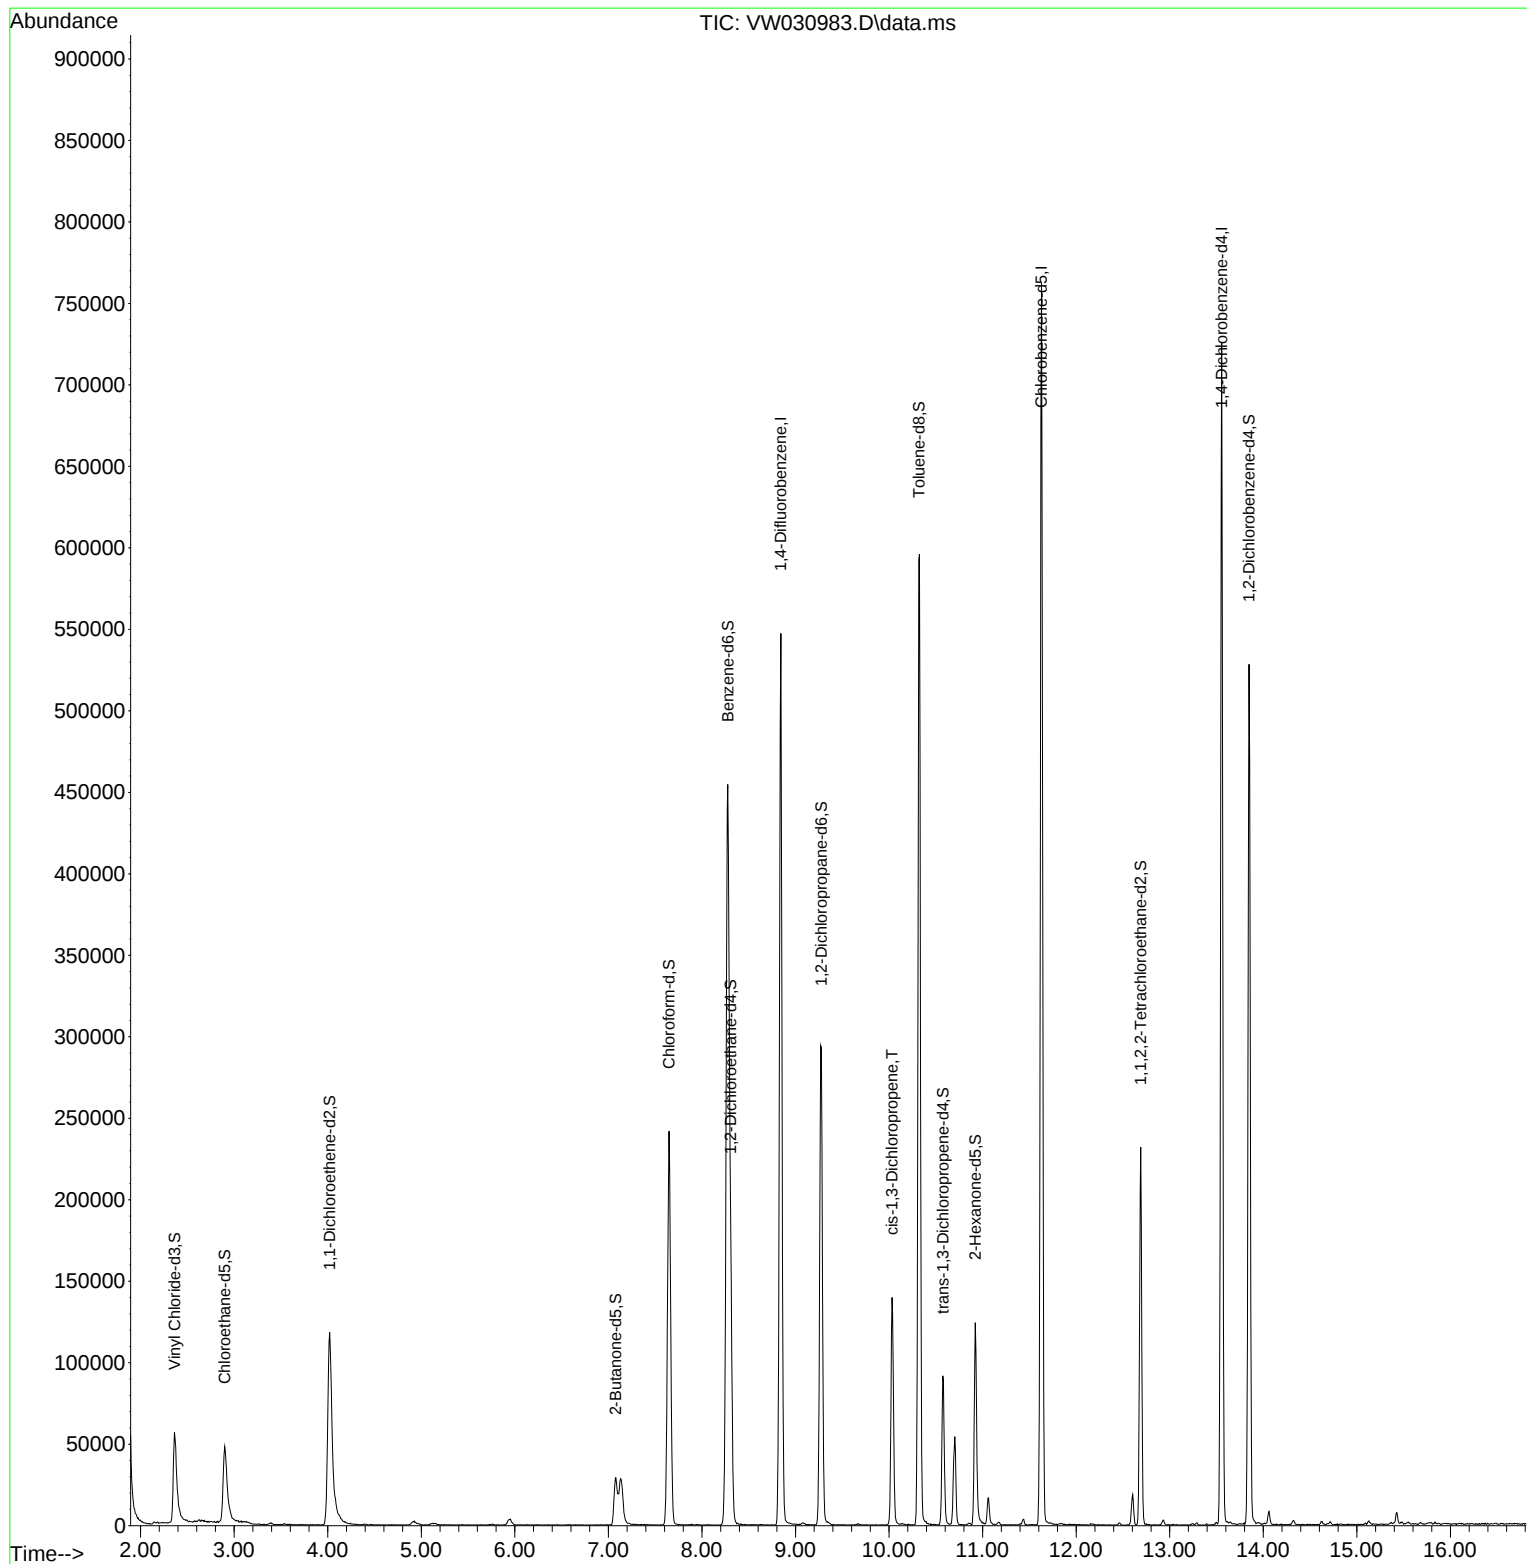

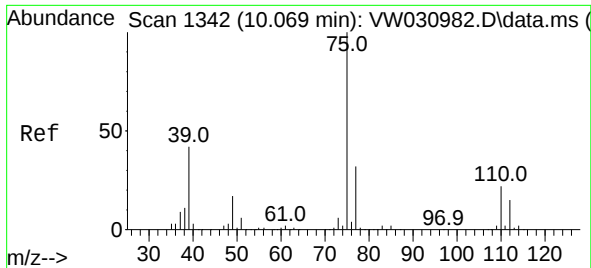

#39
 cis-1,3-Dichloropropene
 Concen: 0.355 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW030983.D
 Acq: 11 Nov 2024 10:40

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3739
 Ion Ratio Lower Upper
 75 100
 77 55.0 21.3 39.6#

