

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111124\
 Data File : VW030987.D
 Acq On : 11 Nov 2024 13:58
 Operator : SY/MD
 Sample : P4724-19
 Misc : 6.53g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 12 00:21:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Nov 12 00:19:56 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	495404	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	432195	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	159729	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	130709	16.087	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.360%
7) Chloroethane-d5	2.899	69	100572	16.139	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.560%
11) 1,1-Dichloroethene-d2	4.027	65	59449	17.732	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.920%
21) 2-Butanone-d5	7.075	46	83283	62.286	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.580%
24) Chloroform-d	7.648	84	285121	19.523	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.080%
26) 1,2-Dichloroethane-d4	8.307	65	151952	20.926	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.720%
32) Benzene-d6	8.276	84	549243	20.456	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.840%
36) 1,2-Dichloropropane-d6	9.270	67	171403	21.655	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.600%
41) Toluene-d8	10.318	98	461582	19.166	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.680%
43) trans-1,3-Dichloroprop...	10.575	79	66023	20.578	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.320%
47) 2-Hexanone-d5	10.922	63	64972	63.337	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.680%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	152881	27.723	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	110.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	132940	22.849	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.400%
Target Compounds			Qvalue			
39) cis-1,3-Dichloropropene	10.038	75	4107	0.394	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111124\
Data File : VW030987.D
Acq On : 11 Nov 2024 13:58
Operator : SY/MD
Sample : P4724-19
Misc : 6.53g/10mL/MSVOA_W/SOIL/B
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 12 00:21:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Nov 12 00:19:56 2024
Response via : Initial Calibration

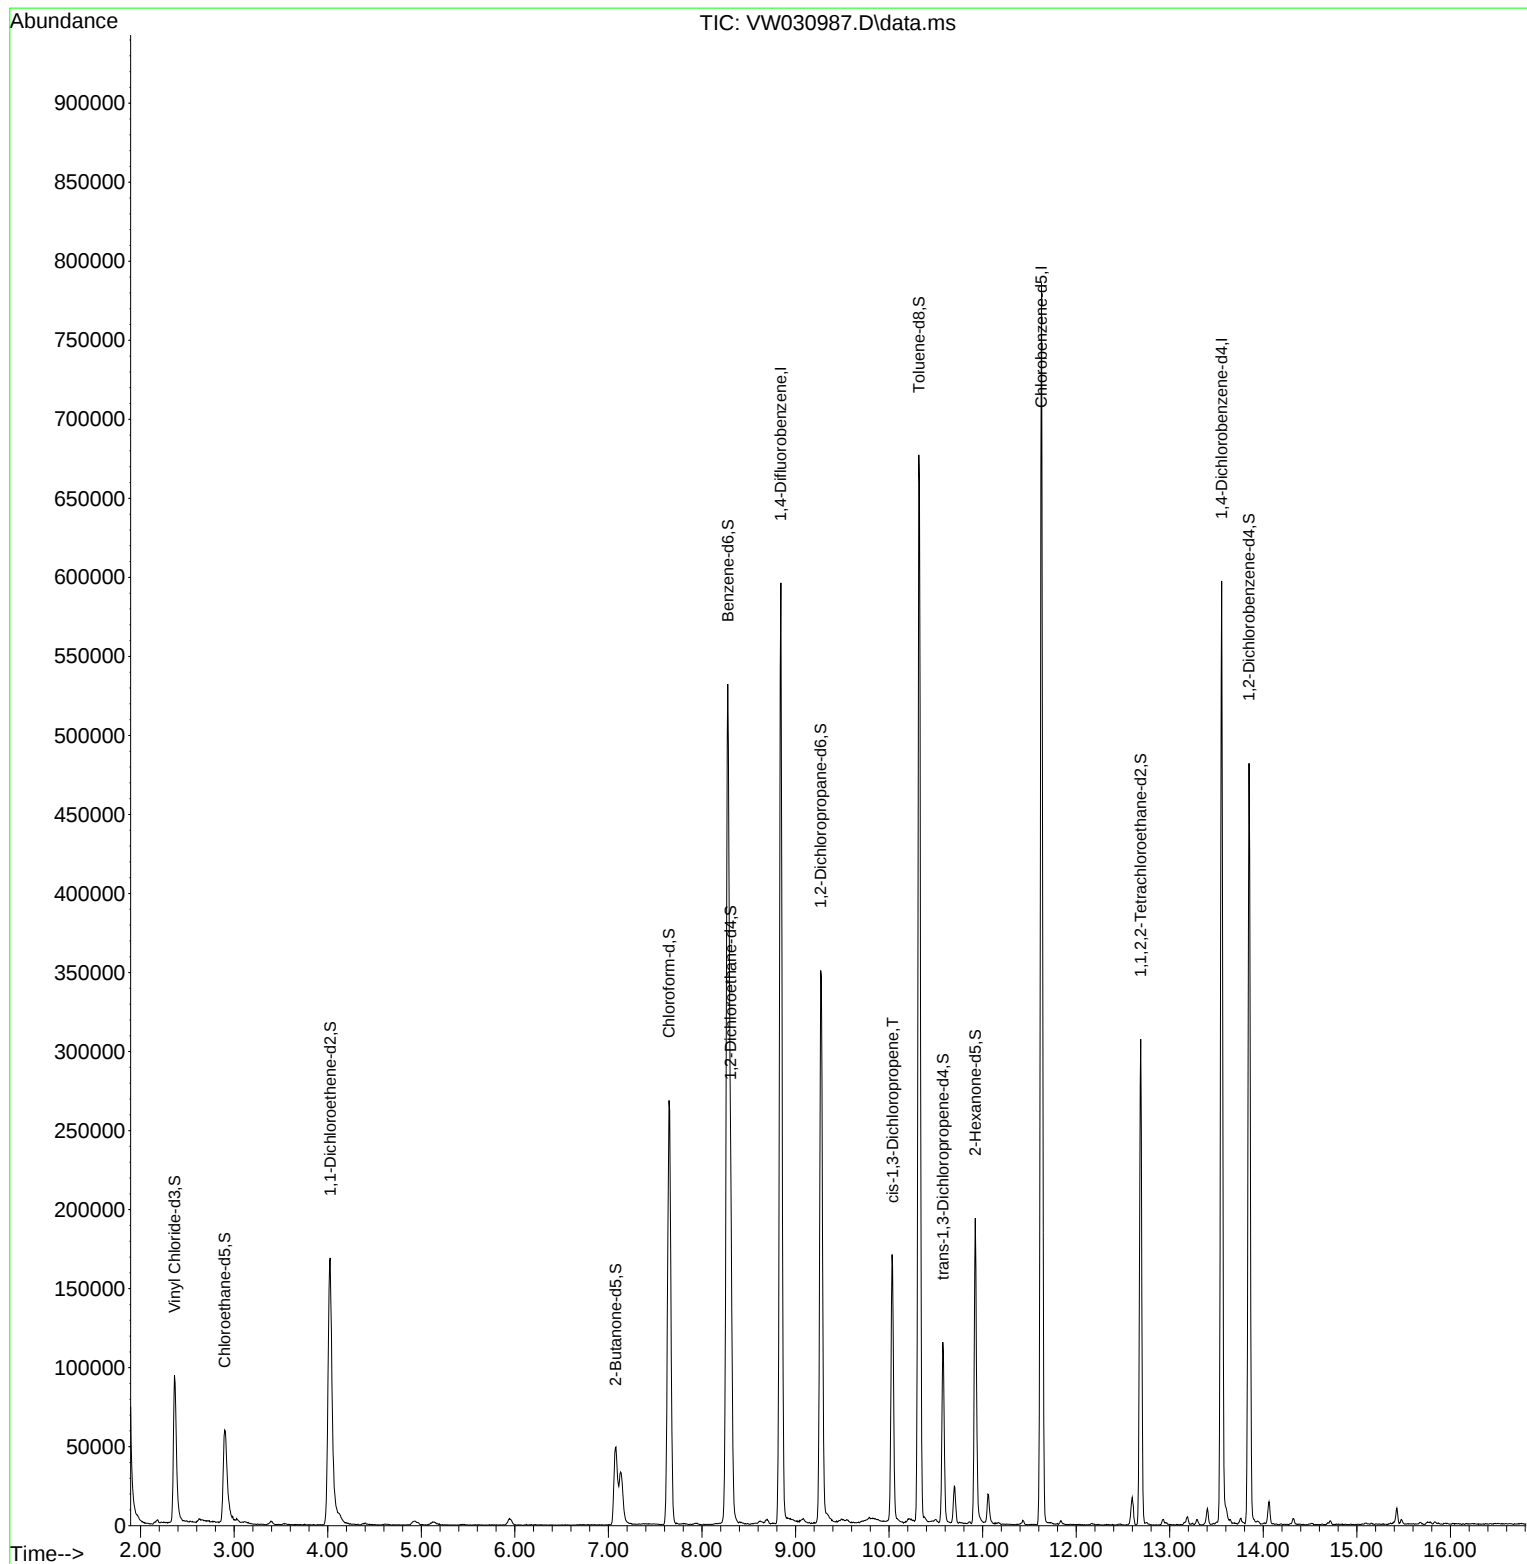

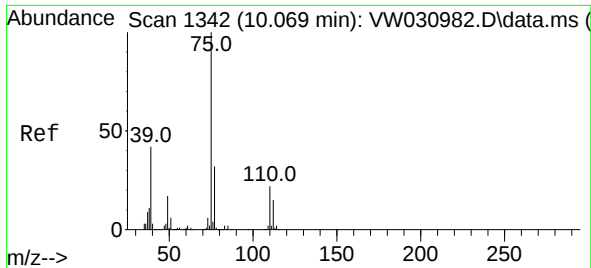

#39
 cis-1,3-Dichloropropene
 Concen: 0.394 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.031 min
 Lab File: VW030987.D
 Acq: 11 Nov 2024 13:58

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4107
 Ion Ratio Lower Upper
 75 100
 77 50.0 21.3 39.6#

