
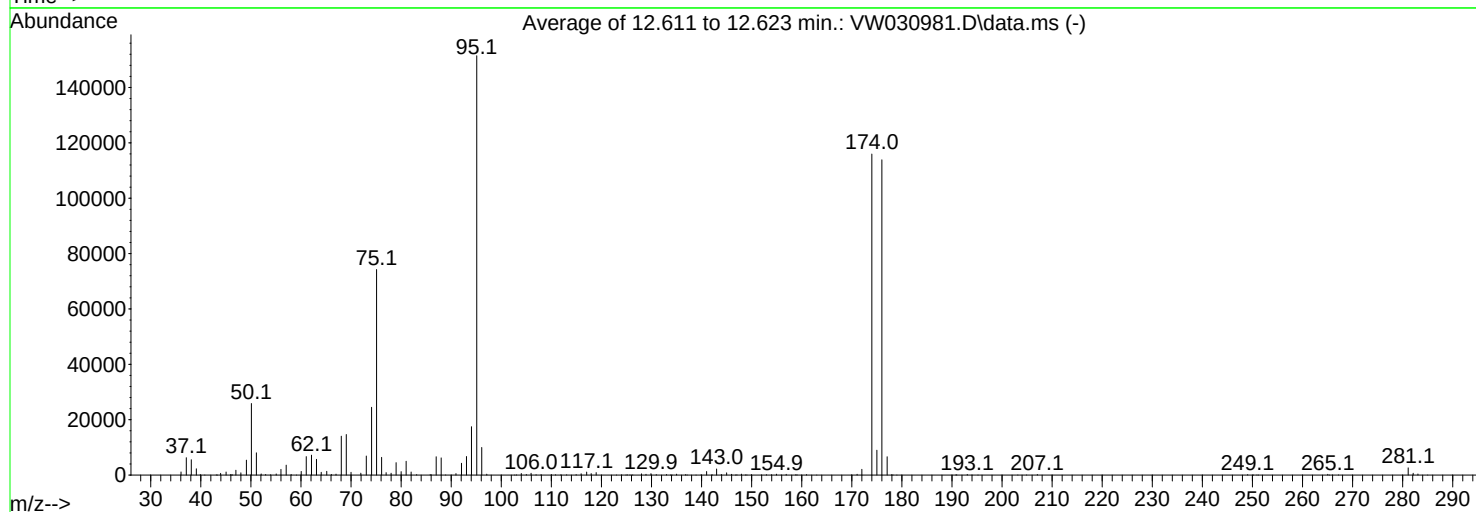


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111124\
Data File : VW030981.D
Acq On : 11 Nov 2024 09:05
Operator : SY/MD
Sample : BFB595
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB595

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Tue Nov 12 00:19:56 2024

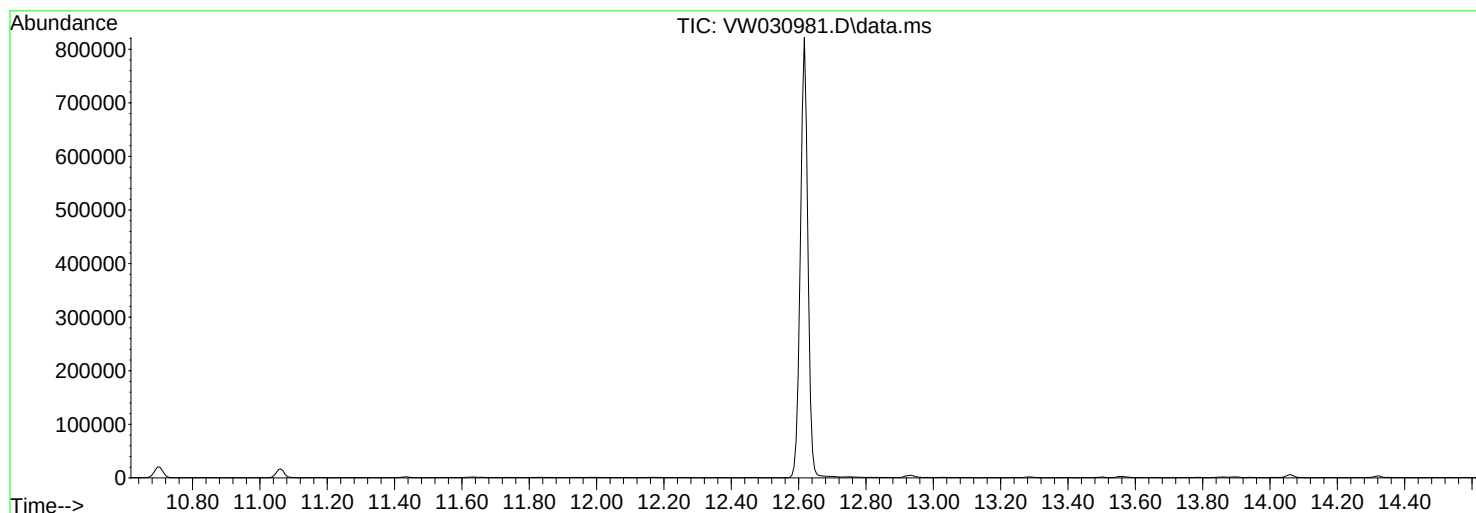

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	25856	PASS
75	95	30	80	49.0	74248	PASS
95	95	100	100	100.0	151467	PASS
96	95	5	9	6.6	9971	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.6	115965	PASS
175	174	5	9	7.8	8991	PASS
176	174	95	101	98.2	113885	PASS
177	176	5	9	5.8	6627	PASS

m/z	Abundance
39.90	195.0
43.90	203.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

m/z	Abundance
36.00	1376.0
37.10	6680.0
38.10	6006.0
39.10	2592.0
39.90	310.0
43.10	114.0
44.00	939.0
45.00	1105.0
46.00	308.0
47.00	1805.0
48.10	999.0
49.10	5280.0
50.10	27696.0
51.10	8474.0
52.00	433.0
53.00	249.0
53.90	93.0
55.10	439.0
56.00	2320.0
57.00	3701.0
58.00	202.0
59.10	82.0
60.10	1255.0
61.00	6856.0
62.10	7659.0
63.10	6179.0
64.00	1079.0
65.10	1397.0
66.10	229.0
67.00	412.0
68.00	14395.0
69.10	14588.0
70.00	1211.0
72.00	646.0
73.10	6875.0
74.10	25024.0
75.10	72824.0
76.10	6695.0
77.00	857.0
78.00	493.0
79.00	4563.0
80.00	1347.0
81.00	5190.0
82.00	1086.0
83.10	139.0
85.80	208.0
87.00	7042.0
88.00	6506.0
91.00	662.0
92.10	4273.0
93.00	6491.0
94.10	16752.0
95.10	144768.0
96.10	9826.0
97.10	424.0
102.70	86.0
103.00	109.0
104.00	557.0
105.10	304.0
105.90	505.0
107.00	200.0
108.10	159.0
110.00	160.0
110.90	110.0
111.90	141.0
113.20	74.0
115.00	200.0
115.90	437.0
117.10	1174.0
117.90	525.0
118.90	924.0
124.10	58.0
125.20	192.0
125.70	132.0
126.20	87.0
128.00	309.0
128.90	338.0
129.90	467.0
131.00	170.0
132.90	308.0
134.10	61.0
135.00	428.0
136.80	260.0
138.90	53.0
141.00	1258.0
142.10	173.0
143.00	2346.0
144.00	301.0
145.00	1010.0
146.00	265.0
147.00	170.0
148.00	255.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

148.80	87.0
149.10	99.0
149.90	112.0
153.00	130.0
153.90	106.0
154.90	353.0
156.90	335.0
158.80	229.0
161.00	156.0
171.00	517.0
172.00	1881.0
174.00	95760.0
175.00	8312.0
176.00	94608.0
177.00	6425.0
177.90	133.0
179.00	92.0
190.80	260.0
193.10	381.0
194.00	63.0
195.20	81.0
203.10	71.0
204.90	55.0
207.10	385.0
249.10	263.0
250.20	65.0
250.90	105.0
265.00	525.0
266.00	65.0
267.20	150.0
281.10	3922.0
282.10	997.0
283.10	645.0
285.00	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

m/z	Abundance
36.10	1207.0
37.10	7315.0
38.10	6015.0
39.10	2573.0
40.00	372.0
40.80	92.0
43.10	101.0
44.00	806.0
45.00	1272.0
45.90	154.0
46.30	240.0
47.00	1983.0
47.90	834.0
49.10	6249.0
50.10	29120.0
51.10	9605.0
52.10	483.0
52.90	194.0
53.90	105.0
55.00	473.0
56.00	2287.0
57.10	4100.0
58.10	170.0
60.00	1580.0
61.10	7570.0
62.10	8245.0
63.10	6129.0
64.10	1254.0
65.10	1591.0
66.10	257.0
67.00	312.0
68.00	15909.0
69.10	17184.0
70.00	1124.0
72.00	850.0
73.10	7897.0
74.10	27992.0
75.10	86280.0
76.10	7514.0
77.00	1078.0
78.00	755.0
79.00	5189.0
80.00	1266.0
81.00	5627.0
82.00	1204.0
83.10	262.0
86.00	288.0
87.00	7377.0
88.00	6709.0
91.00	548.0
92.00	4776.0
93.10	7445.0
94.10	20152.0
95.10	174976.0
96.10	11274.0
97.10	360.0
103.10	112.0
104.00	700.0
104.90	207.0
106.00	805.0
107.00	128.0
107.90	161.0
110.00	208.0
110.90	162.0
111.90	70.0
113.00	118.0
114.90	209.0
115.90	619.0
117.00	1233.0
118.00	666.0
119.00	1131.0
123.00	61.0
124.10	98.0
125.10	120.0
125.70	51.0
126.30	63.0
128.00	560.0
128.90	247.0
129.90	646.0
130.90	160.0
133.00	201.0
133.80	138.0
135.00	289.0
137.10	236.0
139.90	101.0
140.90	1309.0
142.10	204.0
143.00	2535.0
143.90	165.0
145.00	929.0
146.00	269.0
147.10	148.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

148.00	403.0
148.70	133.0
150.00	174.0
151.90	56.0
153.00	175.0
154.00	111.0
155.00	365.0
157.00	281.0
158.80	152.0
159.10	139.0
161.00	182.0
163.00	56.0
170.00	73.0
171.10	372.0
172.00	2745.0
174.00	131072.0
175.00	9792.0
176.00	131392.0
177.00	7032.0
178.00	212.0
191.00	196.0
193.00	277.0
203.20	62.0
204.90	55.0
207.00	187.0
249.00	197.0
251.20	54.0
265.10	304.0
281.10	2681.0
282.10	591.0
283.00	369.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

m/z	Abundance
36.10	815.0
37.10	4836.0
38.10	4614.0
39.10	1656.0
40.00	328.0
43.30	75.0
44.00	768.0
45.10	935.0
46.10	217.0
47.00	1481.0
47.90	604.0
49.10	4658.0
50.10	20752.0
51.10	6059.0
52.00	337.0
53.00	196.0
53.90	69.0
55.00	370.0
56.00	1613.0
57.00	2966.0
58.00	175.0
60.00	1141.0
61.10	5609.0
62.10	5707.0
63.10	4785.0
64.00	713.0
65.20	1091.0
66.00	106.0
67.00	352.0
68.10	11836.0
69.00	12174.0
70.00	683.0
71.90	605.0
73.00	5903.0
74.10	20424.0
75.10	63640.0
76.10	5001.0
77.00	715.0
78.00	807.0
79.00	3744.0
80.00	1164.0
81.00	4173.0
82.00	1036.0
83.10	79.0
85.80	234.0
87.00	5441.0
88.00	5429.0
88.90	158.0
90.90	434.0
92.00	3770.0
93.00	6211.0
94.00	15519.0
95.10	134656.0
96.10	8814.0
97.10	221.0
104.00	483.0
105.00	131.0
106.00	690.0
106.90	114.0
107.90	122.0
110.10	52.0
110.80	95.0
111.90	73.0
112.90	101.0
114.90	131.0
116.00	415.0
117.00	866.0
118.00	436.0
119.00	669.0
123.00	64.0
123.90	67.0
124.90	127.0
128.00	494.0
128.90	309.0
129.90	466.0
131.00	209.0
133.10	123.0
135.00	282.0
136.80	237.0
139.90	120.0
141.10	1308.0
143.00	1756.0
143.90	125.0
144.90	542.0
146.00	312.0
146.80	113.0
147.90	383.0
149.00	108.0
150.00	114.0
152.00	59.0
152.80	124.0
153.90	92.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595

155.00	281.0
155.90	91.0
156.80	218.0
159.00	169.0
160.90	190.0
172.00	1627.0
174.00	121064.0
175.00	8868.0
176.00	115656.0
177.10	6423.0
178.20	202.0
190.90	79.0
192.90	100.0
207.20	58.0
248.90	66.0
265.40	54.0
281.10	1247.0
282.10	413.0
283.20	169.0

Instrument :
MSVOA_W
ClientSampleId :
BFB595