

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
 Data File : VW030992.D
 Acq On : 12 Nov 2024 13:33
 Operator : SY/MD
 Sample : VY1112SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 13 00:28:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 13 00:25:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	421988	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	413230	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	180925	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	113844	16.449	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.800%
7) Chloroethane-d5	2.899	69	98982	18.647	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.600%
11) 1,1-Dichloroethene-d2	4.021	65	56421	19.757	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.040%
21) 2-Butanone-d5	7.075	46	57998	50.922	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.840%
24) Chloroform-d	7.648	84	288669	23.204	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.800%
26) 1,2-Dichloroethane-d4	8.307	65	147198	23.798	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.200%
32) Benzene-d6	8.276	84	554604	21.604	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.400%
36) 1,2-Dichloropropane-d6	9.276	67	170373	22.513	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.040%
41) Toluene-d8	10.325	98	494953	21.495	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.960%
43) trans-1,3-Dichloroprop...	10.574	79	65252	21.271	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.080%
47) 2-Hexanone-d5	10.922	63	49127	50.089	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.180%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	130700	24.789	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.160%
66) 1,2-Dichlorobenzene-d4	13.848	152	174404	26.463	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.840%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	4299	0.432	ug/L	Qvalue # 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
Data File : VW030992.D
Acq On : 12 Nov 2024 13:33
Operator : SY/MD
Sample : VY1112SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 13 00:28:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 13 00:25:58 2024
Response via : Initial Calibration

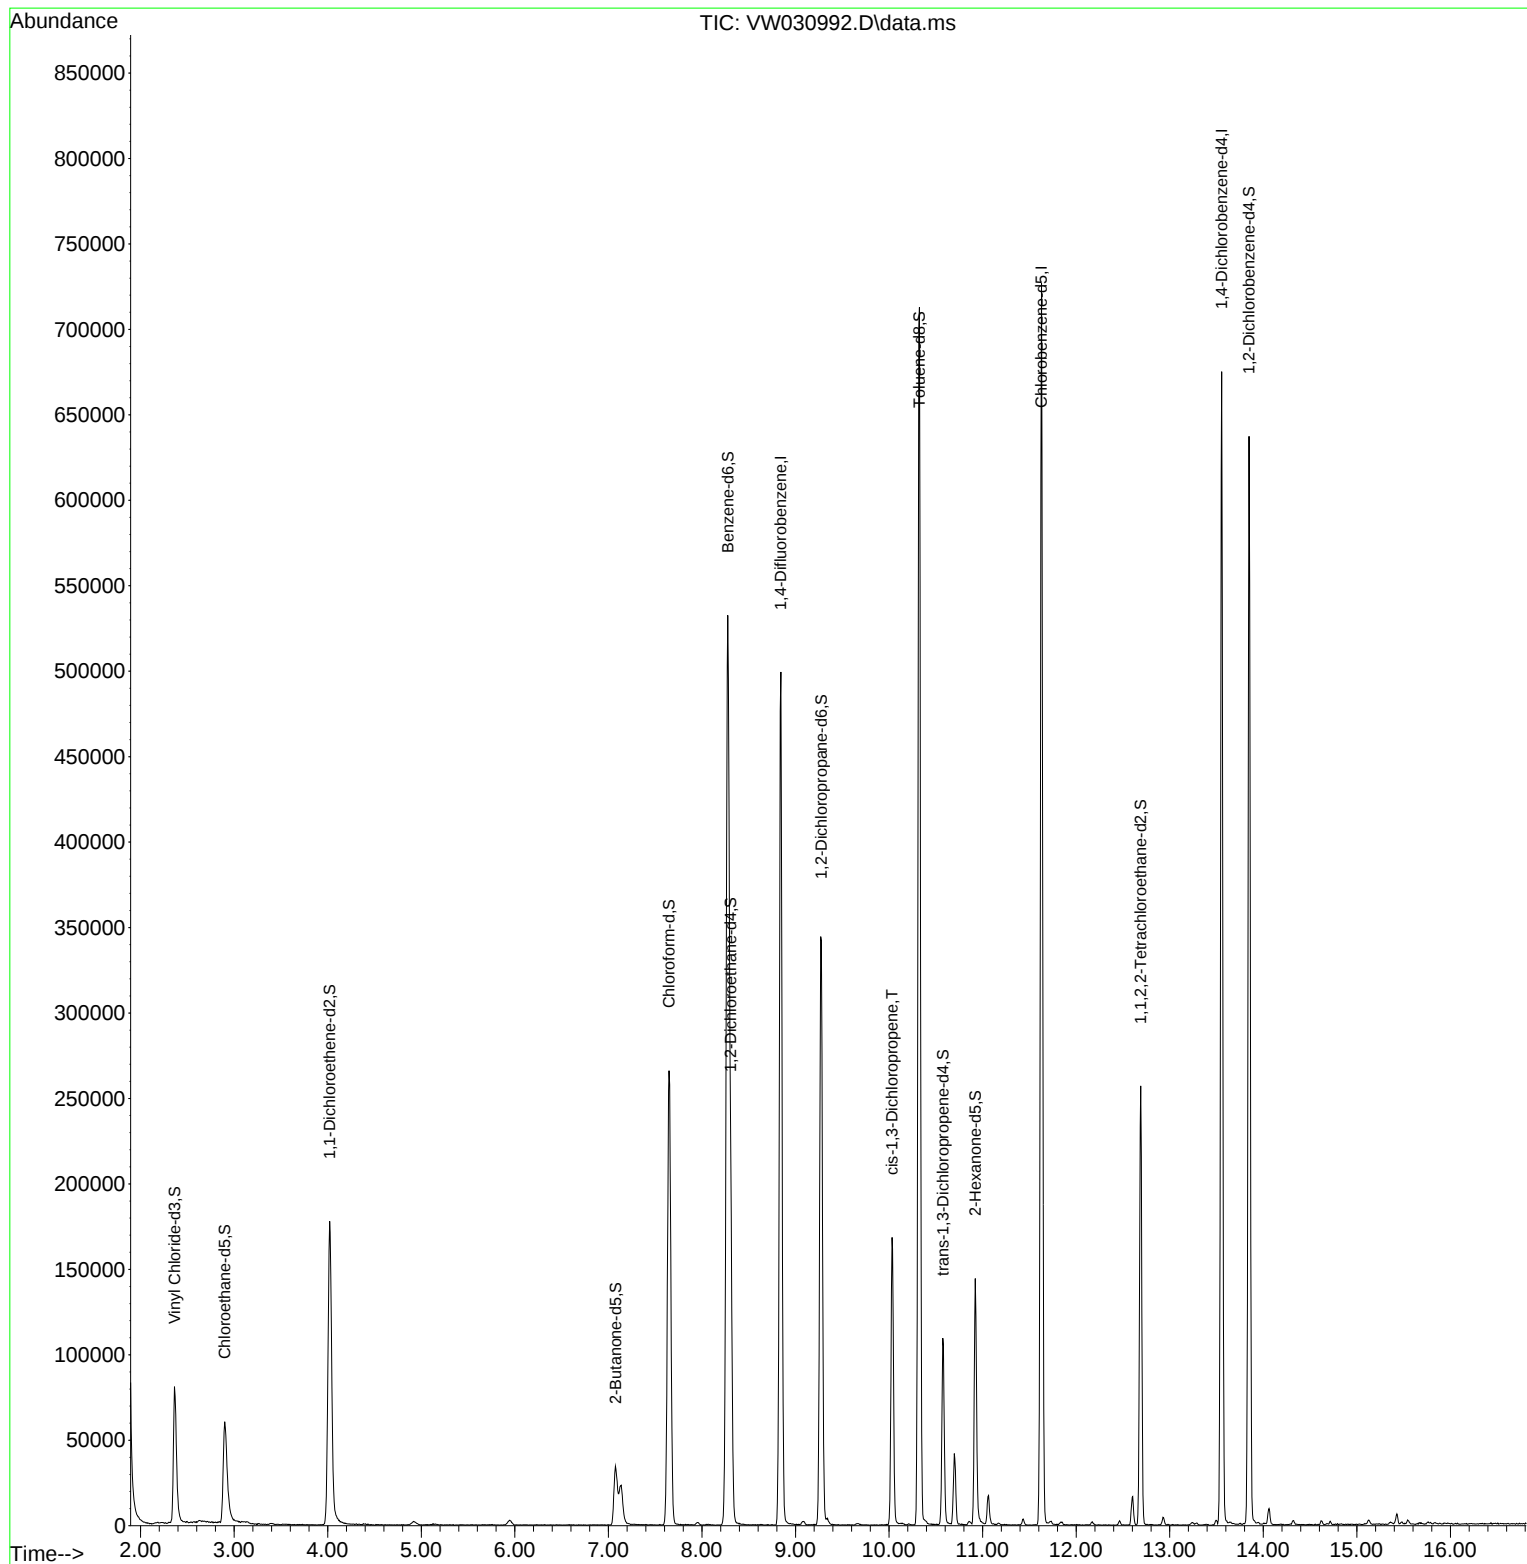

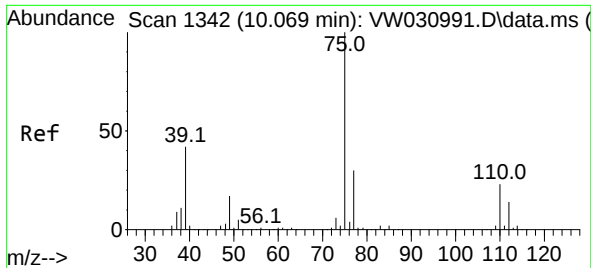

#39
cis-1,3-Dichloropropene
Concen: 0.432 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW030992.D
Acq: 12 Nov 2024 13:33

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 4299
Ion Ratio Lower Upper
75 100
77 51.1 21.3 39.6#

