

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
 Data File : VW030994.D
 Acq On : 12 Nov 2024 14:50
 Operator : SY/MD
 Sample : P4751-14
 Misc : 6.05g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 13 00:28:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 13 00:25:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	512290	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	432974	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	171884	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	116631	13.881	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.520%
7) Chloroethane-d5	2.899	69	97627	15.150	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.600%
11) 1,1-Dichloroethene-d2	4.021	65	52060	15.016	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.080%
21) 2-Butanone-d5	7.075	46	67389	48.738	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.480%
24) Chloroform-d	7.648	84	293505	19.434	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.720%
26) 1,2-Dichloroethane-d4	8.307	65	155883	20.760	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.040%
32) Benzene-d6	8.276	84	520072	19.335	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.320%
36) 1,2-Dichloropropane-d6	9.270	67	174394	21.993	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.960%
41) Toluene-d8	10.324	98	412841	17.111	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.440%
43) trans-1,3-Dichloroprop...	10.574	79	63876	19.873	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.480%
47) 2-Hexanone-d5	10.922	63	53131	51.701	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.400%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	144276	26.116	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.480%
66) 1,2-Dichlorobenzene-d4	13.848	152	135606	21.659	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.640%
Target Compounds						Qvalue
34) Trichloroethene	8.837	95	15237	1.980	ug/L	# 4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
Data File : VW030994.D
Acq On : 12 Nov 2024 14:50
Operator : SY/MD
Sample : P4751-14
Misc : 6.05g/10mL/MSVOA_W/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 13 00:28:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 13 00:25:58 2024
Response via : Initial Calibration

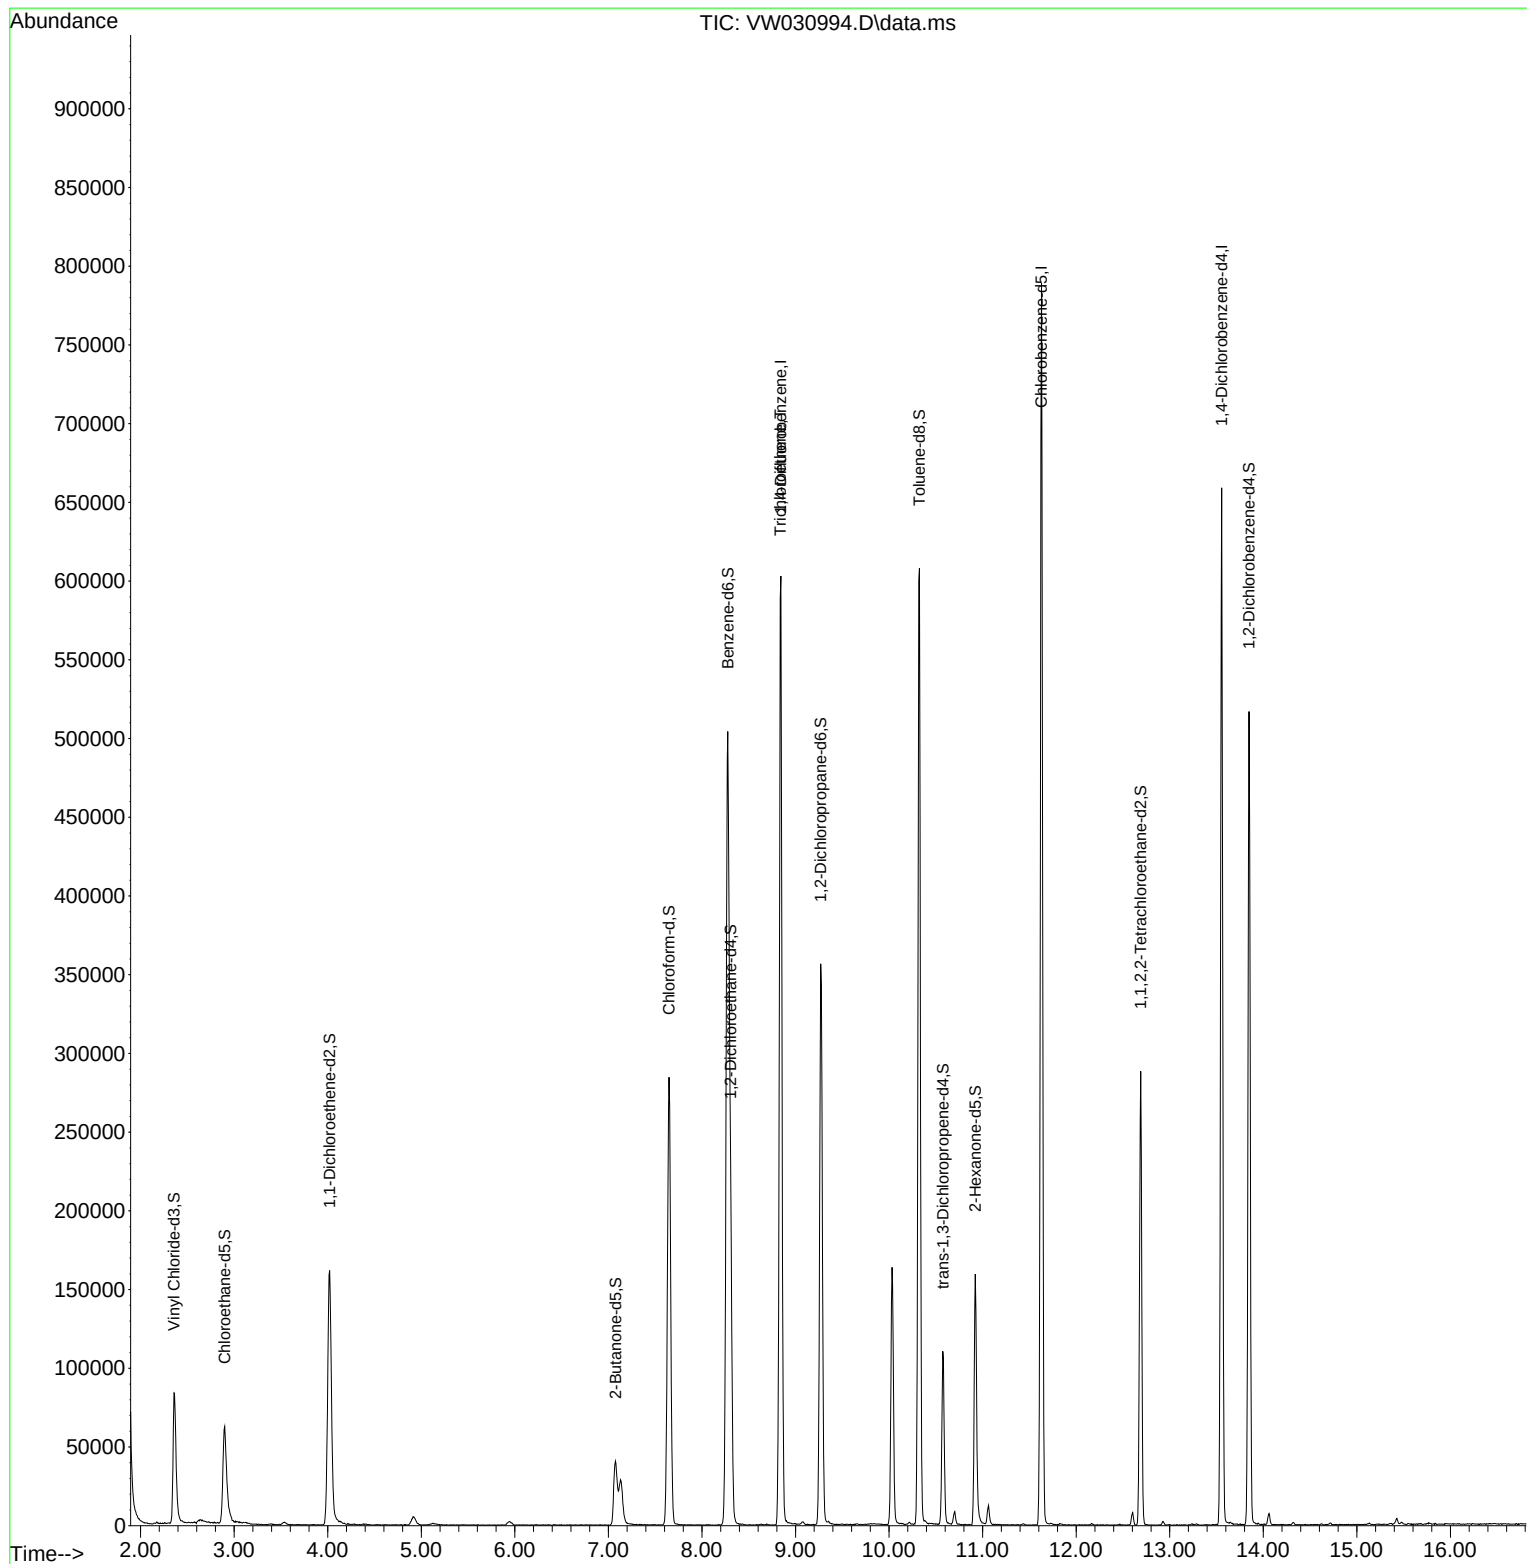

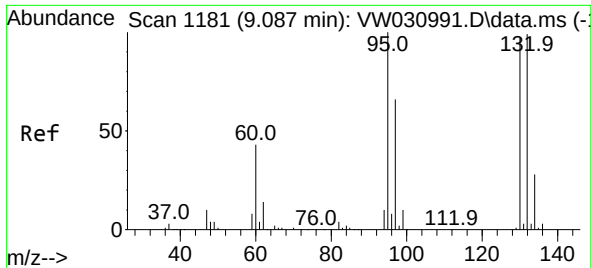

#34
 Trichloroethene
 Concen: 1.980 ug/L
 RT: 8.837 min Scan# 11
 Delta R.T. -0.250 min
 Lab File: VW030994.D
 Acq: 12 Nov 2024 14:50

Instrument :
 MSVOA_W
 ClientSampleId :

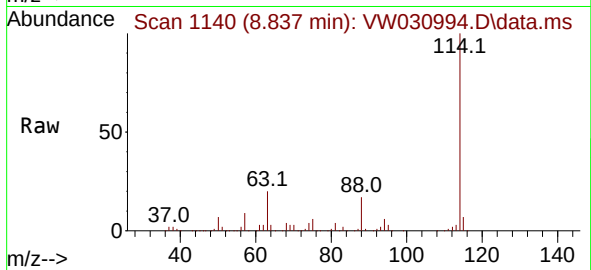

Tgt Ion: 95	Resp: 15237
Ion Ratio	Lower Upper
95	100
97	0.0 48.9 90.7#
132	0.0 67.7 125.7#
130	0.0 73.1 135.8#

