

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
 Data File : VW030998.D
 Acq On : 12 Nov 2024 16:26
 Operator : SY/MD
 Sample : P4751-19
 Misc : 6.72g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 13 00:29:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 13 00:25:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	413346	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	351469	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	128161	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	100675	14.850	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.400%
7) Chloroethane-d5	2.899	69	83312	16.023	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.080%
11) 1,1-Dichloroethene-d2	4.015	65	42923	15.344	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.360%
21) 2-Butanone-d5	7.075	46	74617	66.884	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	133.760%
24) Chloroform-d	7.648	84	257252	21.111	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.440%
26) 1,2-Dichloroethane-d4	8.307	65	143677	23.714	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.840%
32) Benzene-d6	8.270	84	447295	20.485	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.960%
36) 1,2-Dichloropropane-d6	9.270	67	154704	24.034	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.120%
41) Toluene-d8	10.325	98	337336	17.224	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.880%
43) trans-1,3-Dichloroprop...	10.575	79	59155	22.672	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.680%
47) 2-Hexanone-d5	10.922	63	59506	71.332	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	142.660%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	146263	32.615	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	130.440%#
66) 1,2-Dichlorobenzene-d4	13.848	152	112221	24.038	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.160%
Target Compounds						Qvalue
34) Trichloroethene	8.843	95	12650	2.025	ug/L	# 4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
Data File : VW030998.D
Acq On : 12 Nov 2024 16:26
Operator : SY/MD
Sample : P4751-19
Misc : 6.72g/10mL/MSVOA_W/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 13 00:29:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 13 00:25:58 2024
Response via : Initial Calibration

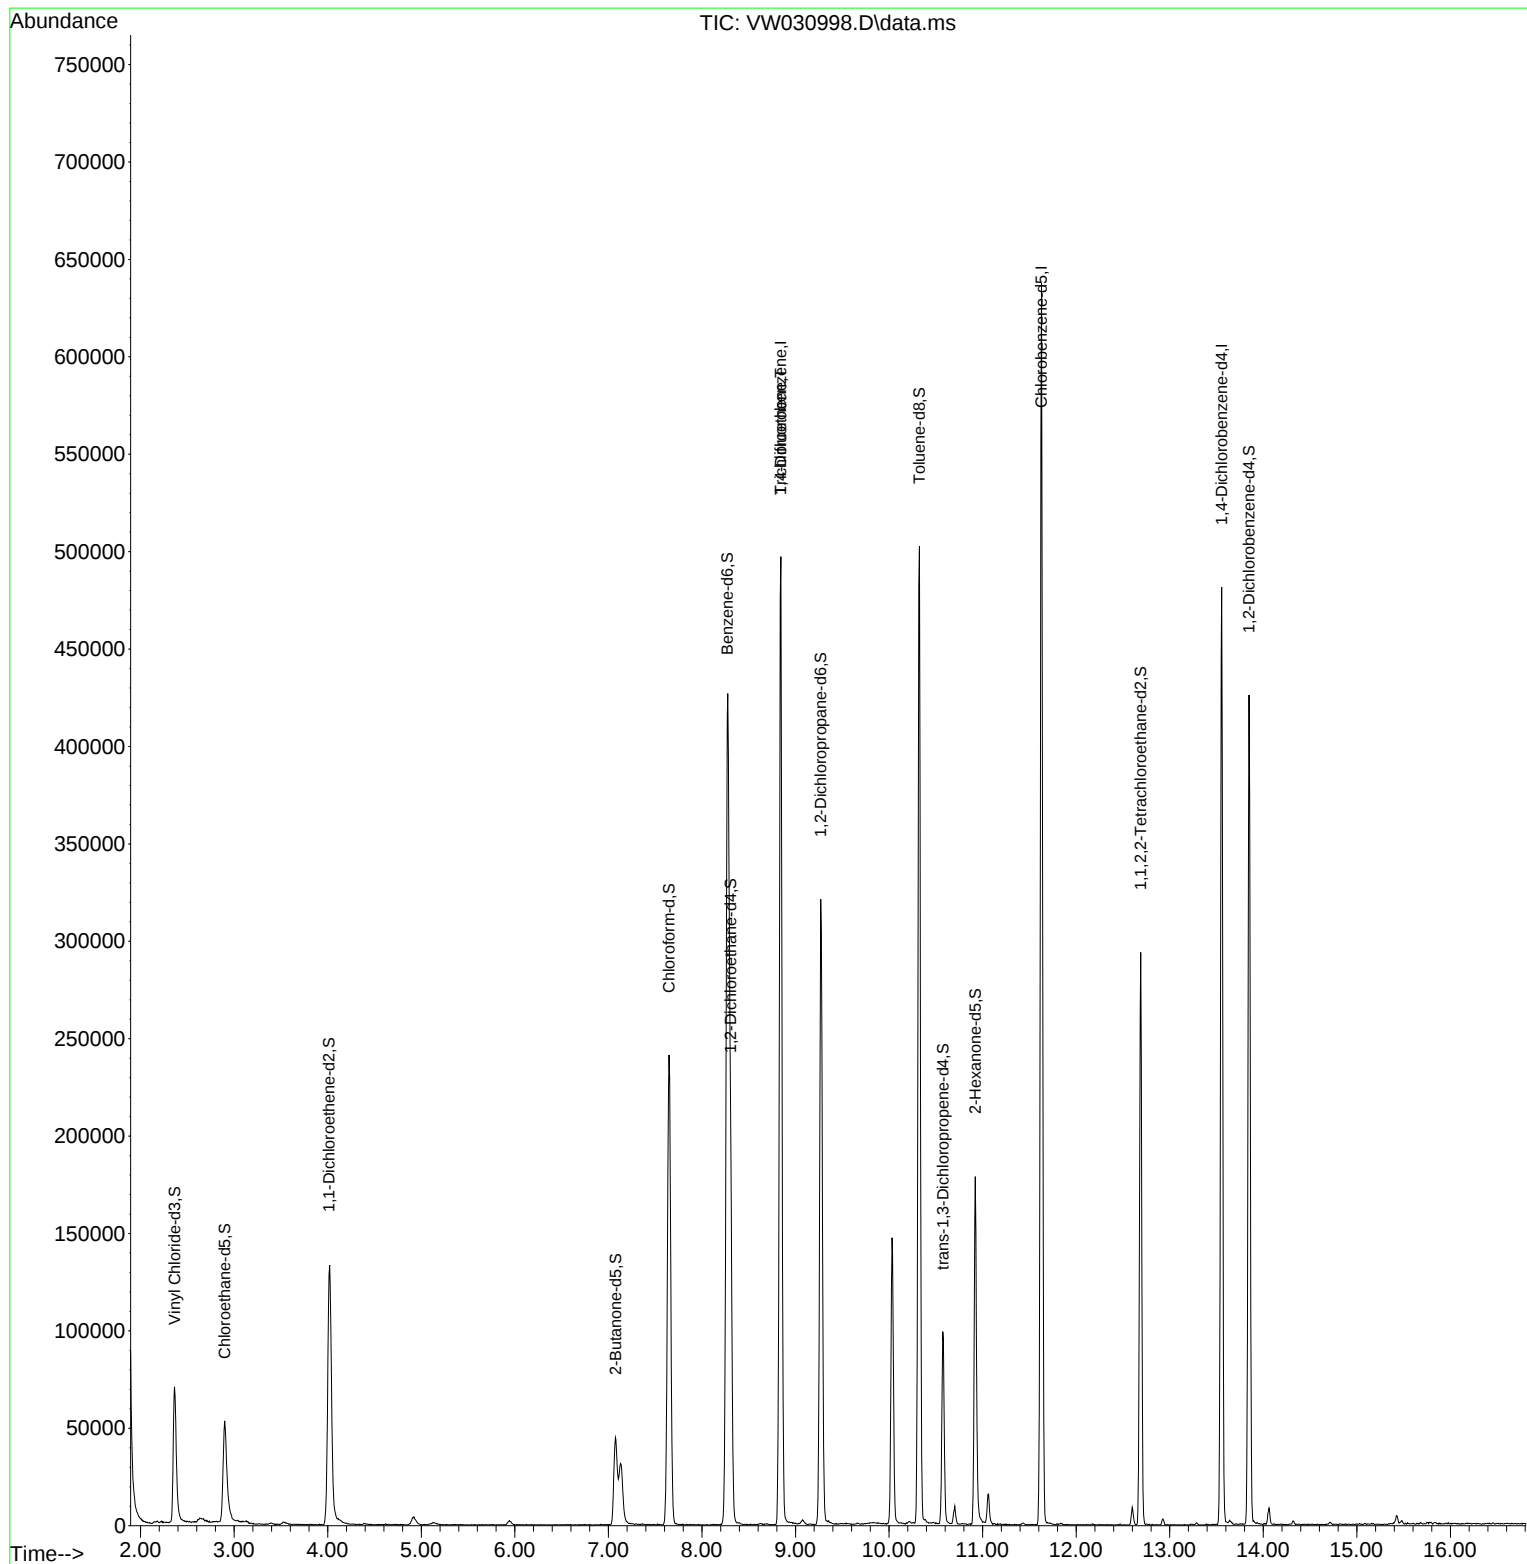

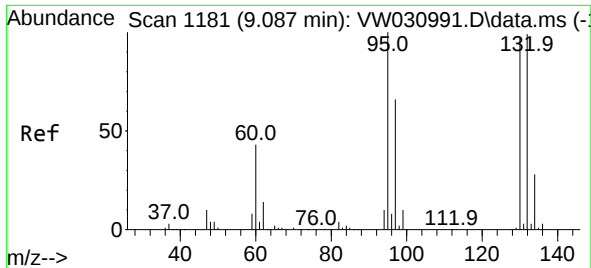

#34
 Trichloroethene
 Concen: 2.025 ug/L
 RT: 8.843 min Scan# 11
 Delta R.T. -0.244 min
 Lab File: VW030998.D
 Acq: 12 Nov 2024 16:26

Instrument :
 MSVOA_W
 ClientSampleId :

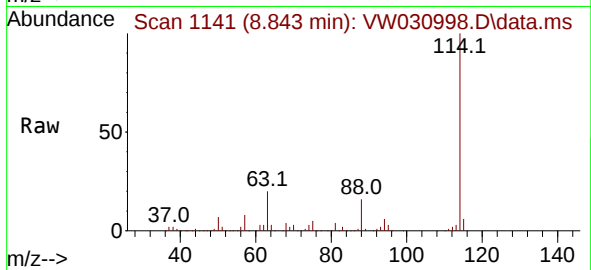

Tgt Ion: 95	Resp: 12650
Ion Ratio	Lower Upper
95 100	
97 0.0	48.9 90.7#
132 0.0	67.7 125.7#
130 0.0	73.1 135.8#

