

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
 Data File : VW031001.D
 Acq On : 12 Nov 2024 17:38
 Operator : SY/MD
 Sample : P4751-22
 Misc : 6.05g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 13 00:30:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 13 00:25:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	349591	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	254901	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	71133	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	114410	19.954	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.800%
7) Chloroethane-d5	2.899	69	88675	20.165	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.680%
11) 1,1-Dichloroethene-d2	4.021	65	46508	19.658	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.640%
21) 2-Butanone-d5	7.075	46	88462	93.755	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	187.500%#
24) Chloroform-d	7.648	84	247382	24.004	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.000%
26) 1,2-Dichloroethane-d4	8.307	65	147338	28.754	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	115.000%
32) Benzene-d6	8.270	84	419160	26.469	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.880%
36) 1,2-Dichloropropane-d6	9.276	67	150264	32.188	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	128.760%#
41) Toluene-d8	10.325	98	281562	19.823	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.280%
43) trans-1,3-Dichloroprop...	10.581	79	54324	28.709	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	114.840%
47) 2-Hexanone-d5	10.922	63	71125	117.561	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	235.120%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	157514	48.430	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	193.720%#
66) 1,2-Dichlorobenzene-d4	13.848	152	78246	30.198	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	120.800%#
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3289	0.535	ug/L	# 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
Data File : VW031001.D
Acq On : 12 Nov 2024 17:38
Operator : SY/MD
Sample : P4751-22
Misc : 6.05g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 13 00:30:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 13 00:25:58 2024
Response via : Initial Calibration

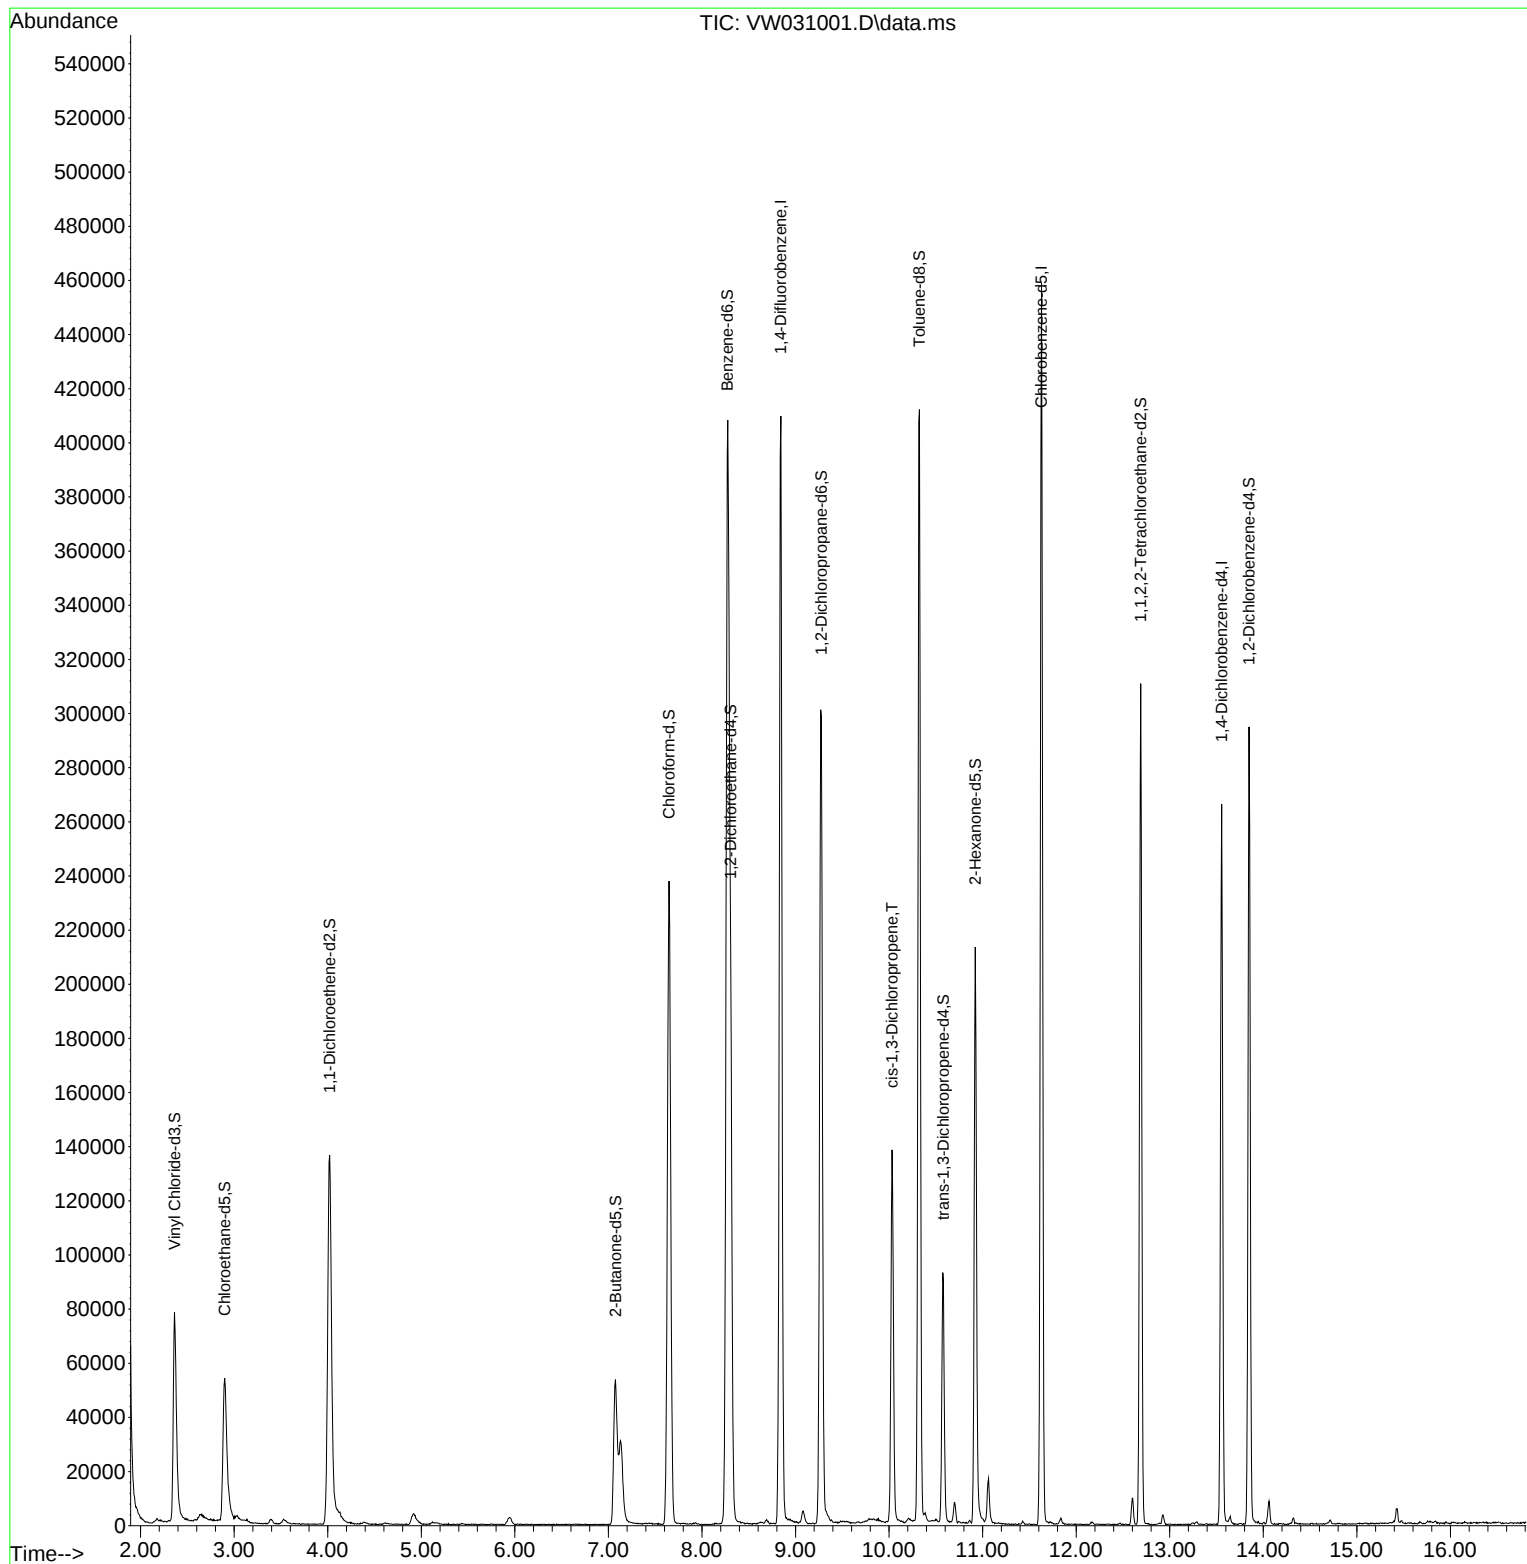

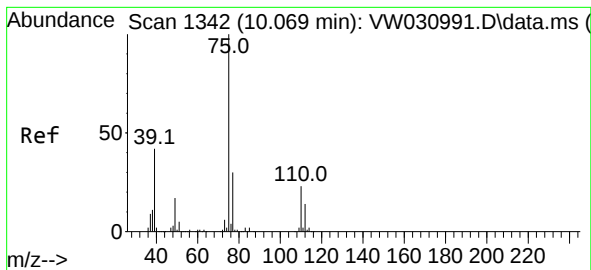

#39
cis-1,3-Dichloropropene
Concen: 0.535 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW031001.D
Acq: 12 Nov 2024 17:38

Instrument :
MSVOA_W
ClientSampleId :

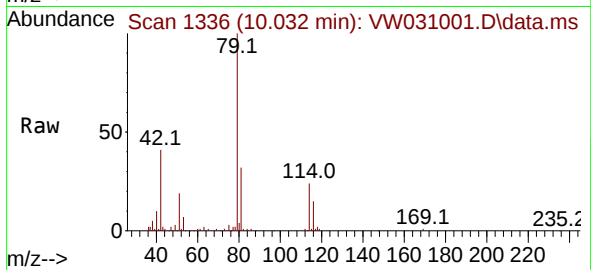

Tgt Ion: 75 Resp: 3289
Ion Ratio Lower Upper
75 100
77 60.5 21.3 39.6#

