
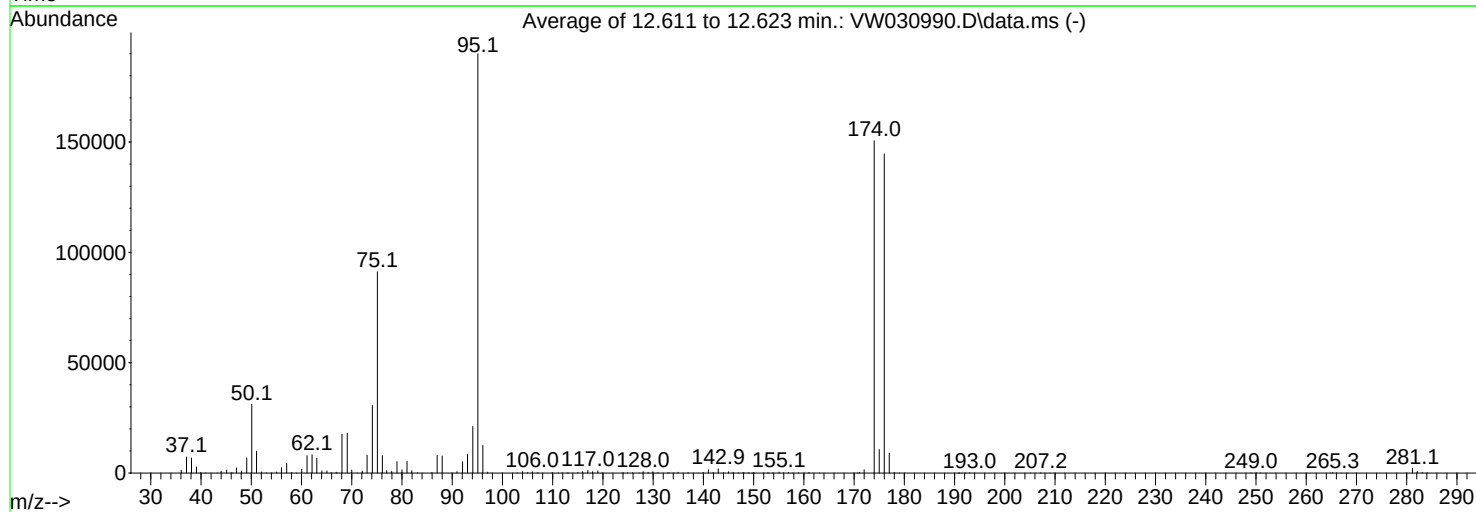


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111224\
Data File : VW030990.D
Acq On : 12 Nov 2024 11:11
Operator : SY/MD
Sample : BFB596
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB596

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Wed Nov 13 00:25:58 2024

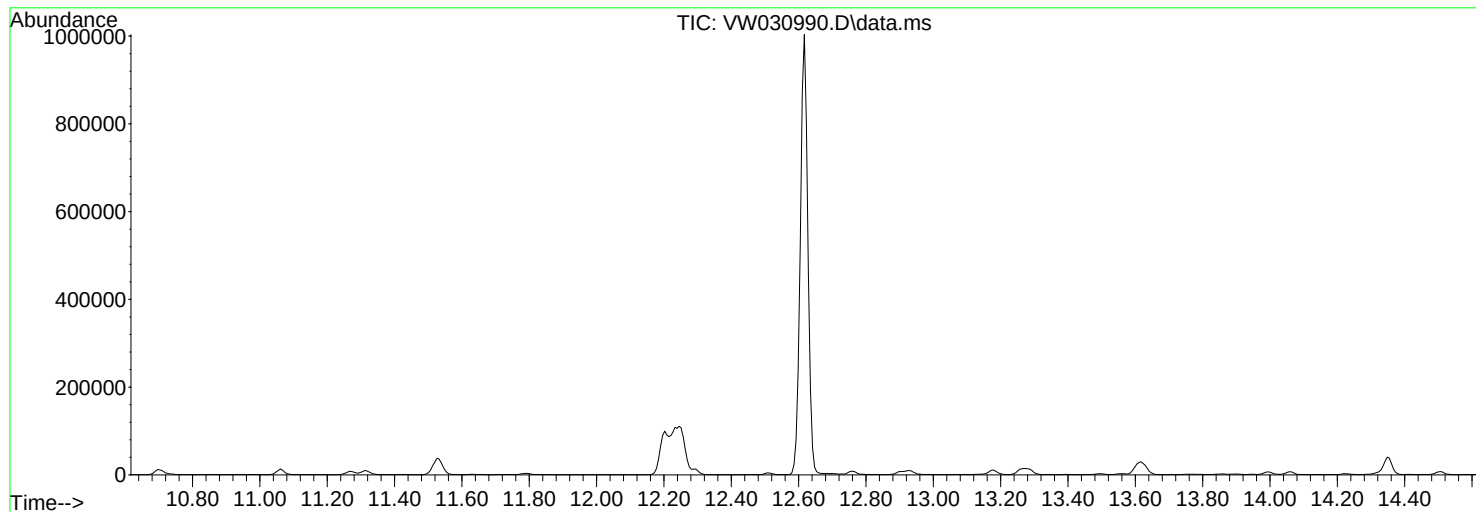

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	31195	PASS
75	95	30	80	48.0	91235	PASS
95	95	100	100	100.0	190016	PASS
96	95	5	9	6.6	12524	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.3	150613	PASS
175	174	5	9	7.0	10610	PASS
176	174	95	101	96.0	144648	PASS
177	176	5	9	6.3	9056	PASS

m/z	Abundance
40.00	328.0
44.00	268.0

Instrument :
MSVOA_W
ClientSampleId :
BFB596

m/z	Abundance
36.00	1504.0
37.10	7605.0
38.10	6889.0
39.10	2741.0
39.90	252.0
41.00	103.0
43.20	96.0
44.10	1082.0
45.10	1537.0
46.00	230.0
47.00	2419.0
48.00	1077.0
49.10	7325.0
50.10	33944.0
51.10	11221.0
52.00	501.0
53.10	169.0
54.10	65.0
55.00	439.0
56.00	2603.0
57.00	4828.0
58.10	220.0
59.00	161.0
60.00	1923.0
61.10	8334.0
62.10	8324.0
63.10	6842.0
64.10	1178.0
65.00	1312.0
65.80	164.0
66.90	591.0
68.10	18408.0
69.10	18632.0
70.00	1348.0
71.10	127.0
72.10	851.0
73.10	8518.0
74.10	30880.0
75.10	90264.0
76.10	7960.0
76.90	1045.0
77.90	909.0
79.00	5236.0
80.00	1546.0
81.00	5104.0
81.90	1108.0
83.10	138.0
86.10	239.0
87.00	8606.0
88.00	7804.0
90.90	690.0
92.10	5070.0
93.00	8027.0
94.10	20048.0
95.10	189504.0
96.10	12293.0
97.10	381.0
102.90	193.0
104.00	746.0
105.00	200.0
106.00	462.0
106.90	161.0
109.90	182.0
111.10	131.0
111.90	104.0
113.00	166.0
115.00	311.0
115.90	674.0
117.00	1168.0
117.90	752.0
119.00	981.0
119.80	64.0
123.90	141.0
124.90	263.0
125.90	97.0
127.20	61.0
128.00	616.0
129.00	331.0
129.90	677.0
130.90	201.0
132.80	234.0
133.20	208.0
134.20	84.0
134.90	410.0
136.90	326.0
138.90	91.0
140.00	152.0
141.00	1434.0
141.90	205.0
142.90	2075.0
144.00	184.0
145.00	826.0

Instrument :
MSVOA_W
ClientSampleId :
BFB596

145.90	431.0
147.00	178.0
147.90	380.0
149.00	155.0
150.00	229.0
152.10	64.0
152.80	133.0
153.80	141.0
155.10	407.0
155.90	61.0
157.00	329.0
159.00	202.0
161.00	362.0
163.10	89.0
171.00	480.0
172.00	1830.0
174.00	139520.0
175.00	10572.0
176.00	125272.0
177.00	8264.0
178.00	295.0
179.10	85.0
190.80	260.0
192.20	57.0
193.10	352.0
194.00	107.0
205.10	78.0
207.10	259.0
209.00	51.0
249.00	263.0
250.10	97.0
250.90	106.0
264.80	170.0
265.30	357.0
266.10	125.0
267.00	93.0
268.30	58.0
280.00	76.0
281.10	2928.0
282.10	1173.0
283.10	468.0
284.20	102.0

Instrument :
MSVOA_W
ClientSampleId :
BFB596

m/z	Abundance
36.10	1443.0
37.10	8337.0
38.10	8419.0
39.10	3477.0
40.10	301.0
40.90	66.0
44.00	1265.0
45.10	1534.0
46.20	272.0
47.10	2706.0
48.10	996.0
49.10	7776.0
50.10	34512.0
51.10	10664.0
52.10	558.0
52.90	139.0
54.10	162.0
55.10	500.0
56.00	2714.0
57.10	5003.0
58.00	177.0
60.10	1895.0
61.10	8624.0
62.10	9375.0
63.10	7961.0
64.00	1049.0
65.00	947.0
65.90	160.0
66.90	624.0
68.10	20304.0
69.10	20088.0
70.00	1623.0
72.10	1094.0
73.10	9334.0
74.10	34392.0
75.10	105248.0
76.10	8949.0
77.00	1218.0
78.00	874.0
79.00	5834.0
80.00	1638.0
81.00	6339.0
82.00	1158.0
82.90	93.0
83.20	95.0
85.90	223.0
87.00	9444.0
88.00	9048.0
91.00	736.0
92.10	5430.0
93.10	9361.0
94.10	24352.0
95.10	211392.0
96.10	14151.0
97.00	515.0
102.90	100.0
104.00	647.0
105.00	326.0
105.90	753.0
107.10	178.0
109.90	148.0
111.10	175.0
112.00	163.0
112.80	192.0
115.10	212.0
115.90	758.0
117.00	1234.0
118.00	701.0
119.00	1188.0
119.80	57.0
124.10	125.0
125.00	128.0
125.90	85.0
127.20	72.0
128.00	690.0
129.00	384.0
130.00	729.0
131.00	233.0
133.10	291.0
134.10	60.0
135.00	580.0
137.00	325.0
139.00	112.0
139.90	171.0
141.00	1581.0
141.90	245.0
143.00	2297.0
144.00	138.0
145.00	559.0
145.90	359.0
147.00	187.0
147.90	501.0

Instrument :
MSVOA_W
ClientSampleId :
BFB596

148.80	155.0
149.90	166.0
152.00	63.0
152.80	220.0
153.90	116.0
155.00	621.0
156.00	97.0
157.00	417.0
158.90	192.0
161.00	337.0
163.10	56.0
170.70	178.0
171.10	267.0
172.00	1458.0
174.00	162112.0
175.00	11136.0
176.00	169344.0
177.00	9978.0
178.00	248.0
179.00	80.0
191.00	154.0
192.90	160.0
193.90	59.0
207.20	171.0
248.90	128.0
250.10	64.0
251.00	84.0
265.30	183.0
266.00	99.0
281.20	2411.0
282.10	667.0
283.10	480.0
284.10	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB596

m/z	Abundance
36.10	1072.0
37.10	5897.0
38.10	5187.0
39.00	2072.0
40.00	382.0
40.80	71.0
44.10	882.0
45.10	1094.0
46.00	114.0
47.00	1856.0
48.00	740.0
49.10	5541.0
50.10	25128.0
51.00	7984.0
52.00	447.0
54.10	73.0
55.00	427.0
56.00	2043.0
57.00	3371.0
58.00	187.0
60.00	1348.0
61.10	6724.0
62.10	7041.0
63.00	5444.0
64.10	765.0
65.10	793.0
66.00	147.0
67.10	404.0
68.00	14239.0
69.10	15365.0
70.00	1171.0
72.10	839.0
73.00	6595.0
74.10	26576.0
75.10	78192.0
76.10	6786.0
77.00	1158.0
78.00	741.0
79.00	4500.0
80.00	1264.0
81.00	4477.0
82.00	979.0
83.20	72.0
85.90	288.0
87.10	5926.0
88.00	6416.0
91.00	531.0
92.00	4939.0
93.10	8173.0
94.10	18904.0
95.10	169152.0
96.10	11129.0
97.00	271.0
103.00	145.0
104.00	632.0
105.00	157.0
105.90	596.0
107.10	188.0
109.90	52.0
111.10	100.0
112.00	90.0
113.10	152.0
114.90	218.0
116.00	503.0
117.00	1158.0
118.00	679.0
119.00	876.0
119.90	63.0
123.70	65.0
125.90	106.0
128.00	713.0
129.00	310.0
129.90	591.0
131.00	263.0
133.00	87.0
135.00	230.0
137.00	252.0
139.90	192.0
141.00	1631.0
142.00	234.0
143.00	1553.0
144.00	163.0
144.90	374.0
146.00	213.0
147.00	134.0
148.10	393.0
149.10	144.0
149.70	74.0
150.20	57.0
153.00	210.0
153.90	129.0
155.00	452.0

Instrument :
MSVOA_W
ClientSampleId :
BFB596

156.00	91.0
156.90	268.0
157.70	71.0
159.00	166.0
161.00	218.0
171.00	248.0
172.00	1350.0
174.00	150208.0
175.00	10123.0
176.00	139328.0
177.00	8925.0
178.00	196.0
190.90	122.0
191.40	56.0
192.90	105.0
249.10	92.0
265.10	99.0
281.10	1002.0
282.20	340.0
283.00	153.0
284.20	80.0

Instrument :
MSVOA_W
ClientSampleId :
BFB596