


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111418\
Data File : VW006872.D
Acq On : 14 Nov 2018 12:02
Operator : SY/AP
Sample : BFB81
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB81

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111418S.M
Title : VOC Analysis
Last Update : Wed Nov 14 11:19:19 2018

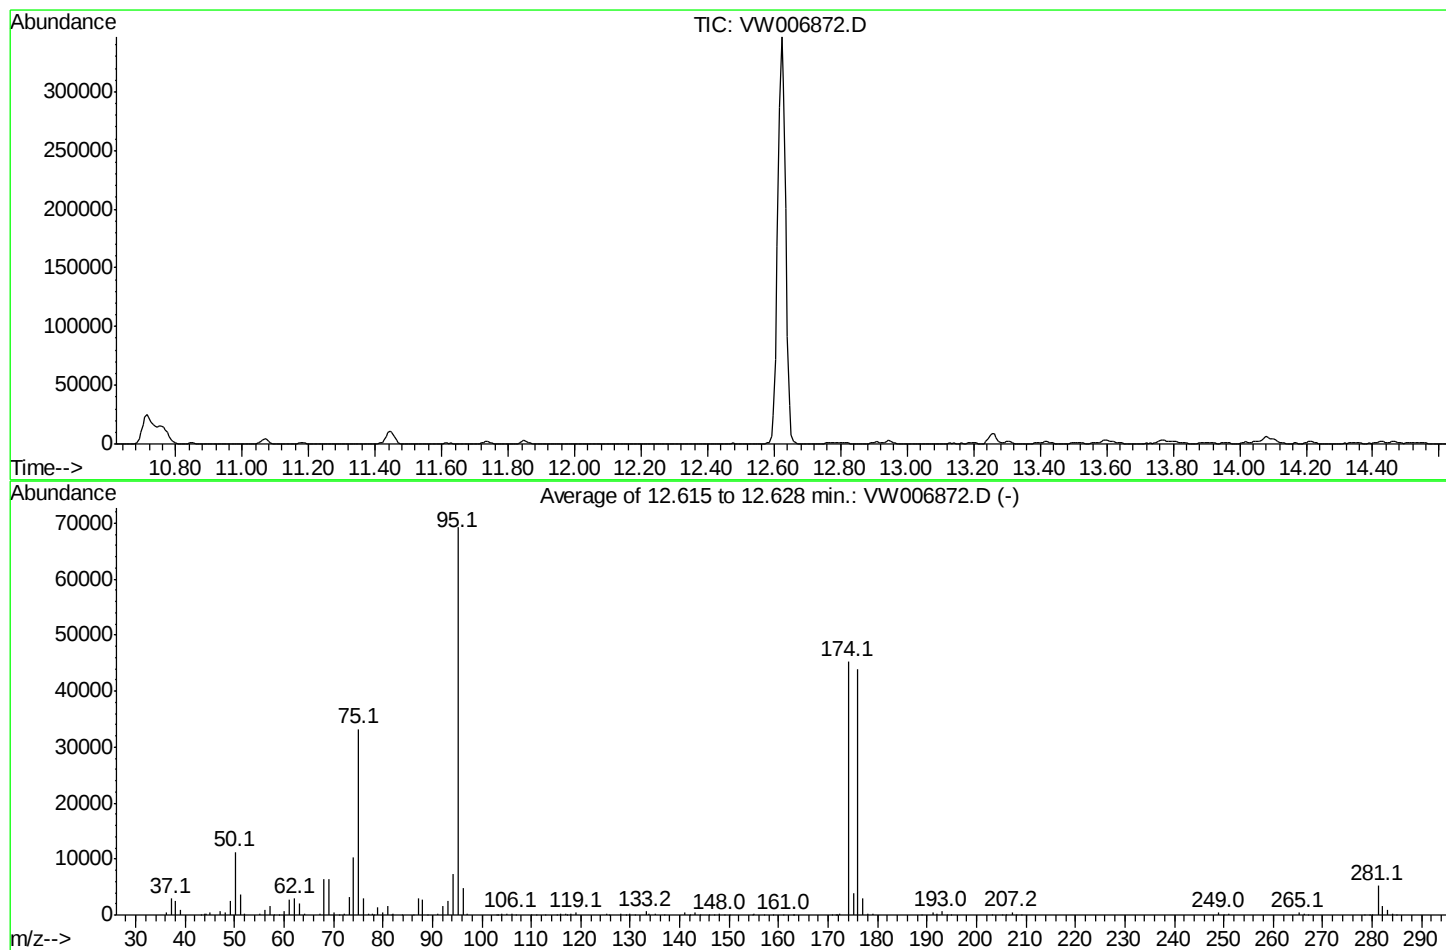

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	11322	PASS
75	95	30	80	48.0	33218	PASS
95	95	100	100	100.0	69261	PASS
96	95	5	9	7.1	4907	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.3	45253	PASS
175	174	5	9	8.6	3879	PASS
176	174	95	101	97.1	43920	PASS
177	176	5	9	6.6	2900	PASS

Scan 1750 (12.573 min): VW006872.D
BFB81

m/z	Abundance
39.90	67.0
41.20	64.0
43.20	98.0
44.10	88.0
55.10	60.0
56.00	53.0
57.20	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

m/z	Abundance
36.10	539.0
37.10	2748.0
38.10	2718.0
39.10	937.0
41.00	63.0
43.00	173.0
44.00	399.0
45.10	636.0
47.20	798.0
48.10	399.0
49.10	2663.0
50.10	10940.0
51.10	3473.0
52.00	187.0
55.10	226.0
56.00	867.0
57.10	1517.0
58.00	106.0
59.10	142.0
60.10	592.0
61.10	2441.0
62.10	2546.0
63.10	1958.0
64.10	169.0
67.20	172.0
68.10	6337.0
69.10	5939.0
70.10	441.0
72.10	366.0
73.10	3026.0
74.10	9728.0
75.10	31304.0
76.10	2941.0
77.20	319.0
77.80	206.0
79.00	1425.0
80.00	369.0
81.00	1380.0
81.80	253.0
87.10	2997.0
88.10	2499.0
91.00	248.0
92.10	1563.0
93.10	2328.0
94.10	6779.0
95.10	63000.0
96.10	4743.0
97.20	139.0
103.00	171.0
104.00	235.0
105.00	149.0
106.00	247.0
106.90	53.0
110.10	89.0
111.00	113.0
112.90	101.0
115.00	73.0
116.10	207.0
116.90	348.0
118.00	250.0
119.10	431.0
125.10	251.0
125.70	73.0
128.00	328.0
129.00	85.0
130.00	202.0
130.90	131.0
133.10	930.0
133.80	213.0
134.90	219.0
140.90	446.0
143.00	519.0
144.20	53.0
145.90	63.0
146.90	109.0
148.00	133.0
149.10	78.0
149.90	121.0
154.80	65.0
155.20	53.0
157.00	108.0
161.00	94.0
162.90	104.0
170.80	80.0
171.80	129.0
174.10	36736.0
175.10	3388.0
176.10	36536.0
177.10	2764.0
178.00	188.0
179.10	155.0
189.10	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

191.10	738.0
192.10	186.0
193.00	868.0
194.10	115.0
203.10	69.0
205.20	127.0
207.10	692.0
208.00	148.0
209.10	74.0
249.00	373.0
250.10	85.0
251.10	135.0
265.20	526.0
266.20	135.0
267.00	130.0
278.30	59.0
279.60	115.0
281.10	6264.0
282.10	1788.0
283.10	1030.0
284.10	176.0
285.00	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

m/z	Abundance
36.10	518.0
37.10	3234.0
38.10	2899.0
39.10	971.0
43.10	90.0
44.20	488.0
45.10	598.0
47.10	973.0
48.00	515.0
49.10	2706.0
50.10	12524.0
51.10	4304.0
52.00	146.0
55.00	218.0
56.10	1057.0
57.10	1844.0
58.00	107.0
59.00	130.0
60.10	634.0
61.10	3463.0
62.10	3245.0
63.10	2140.0
64.10	221.0
67.20	233.0
68.10	7083.0
69.10	7107.0
70.10	579.0
71.30	81.0
72.10	403.0
73.10	3929.0
74.10	10906.0
75.10	36592.0
76.10	3350.0
77.00	407.0
78.20	273.0
79.00	1688.0
80.00	582.0
81.00	1677.0
82.00	349.0
83.90	88.0
86.20	110.0
87.00	3122.0
88.00	3381.0
89.10	52.0
91.10	193.0
92.10	1603.0
93.10	2837.0
94.10	8054.0
95.10	77704.0
96.10	5210.0
97.10	139.0
103.30	171.0
104.00	296.0
105.00	218.0
106.10	256.0
106.90	57.0
110.00	81.0
111.00	149.0
115.00	78.0
116.00	260.0
116.90	392.0
117.90	315.0
119.10	533.0
125.10	235.0
128.00	288.0
129.00	162.0
129.90	260.0
131.00	111.0
133.20	572.0
133.90	264.0
135.00	187.0
137.00	63.0
140.90	592.0
142.00	148.0
142.90	484.0
144.10	78.0
145.90	70.0
147.00	163.0
148.00	223.0
149.00	99.0
150.00	66.0
155.10	135.0
157.00	148.0
158.90	61.0
161.00	145.0
163.10	84.0
170.80	108.0
171.50	101.0
172.20	262.0
174.00	50200.0
175.10	4363.0
176.10	47680.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

177.10	3159.0
178.00	182.0
179.10	162.0
188.90	94.0
191.10	567.0
191.90	105.0
193.00	687.0
194.00	119.0
205.10	133.0
206.00	66.0
207.20	490.0
208.10	107.0
209.20	55.0
249.00	418.0
250.10	78.0
251.10	162.0
265.10	382.0
266.10	119.0
267.10	132.0
279.40	129.0
281.10	5455.0
282.10	1646.0
283.10	1139.0
284.10	175.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

m/z	Abundance
36.10	551.0
37.10	2745.0
38.10	2221.0
39.10	941.0
39.90	91.0
43.00	78.0
44.00	329.0
45.10	488.0
47.00	506.0
48.00	315.0
49.10	2080.0
50.10	10503.0
51.10	3283.0
52.10	141.0
55.00	147.0
56.10	731.0
57.10	1514.0
58.00	76.0
60.10	617.0
61.10	2361.0
62.10	2859.0
63.10	2094.0
64.00	262.0
67.10	196.0
68.10	5677.0
69.10	6287.0
70.00	582.0
71.20	120.0
72.00	268.0
73.10	2832.0
74.10	10194.0
75.10	31760.0
76.10	2567.0
77.00	316.0
77.90	313.0
79.00	1123.0
80.00	321.0
81.00	1516.0
82.10	238.0
83.90	67.0
86.00	154.0
87.00	2732.0
88.00	2576.0
90.90	200.0
92.10	1667.0
93.10	2454.0
94.10	7065.0
95.10	67080.0
96.10	4769.0
97.00	116.0
103.10	95.0
104.00	323.0
105.00	60.0
106.00	206.0
107.00	67.0
110.00	134.0
110.80	78.0
115.00	117.0
115.90	229.0
117.10	316.0
118.10	308.0
118.90	330.0
125.00	153.0
128.00	274.0
129.00	103.0
130.00	230.0
130.80	110.0
133.20	388.0
133.90	77.0
134.90	154.0
136.90	72.0
141.00	470.0
141.90	80.0
143.00	732.0
145.90	57.0
147.00	66.0
148.00	151.0
149.10	53.0
150.00	61.0
155.00	213.0
156.90	79.0
158.90	100.0
161.00	77.0
163.00	71.0
170.80	76.0
171.50	138.0
172.30	300.0
174.10	48824.0
175.10	3887.0
176.00	47544.0
177.00	2779.0
178.00	142.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81

179.20	76.0
188.80	75.0
191.10	403.0
192.10	196.0
193.00	505.0
194.10	59.0
194.90	73.0
205.10	70.0
207.20	386.0
249.00	312.0
250.00	64.0
251.00	76.0
265.10	312.0
266.10	163.0
267.00	63.0
279.40	93.0
280.10	237.0
281.20	3989.0
282.20	1374.0
283.20	649.0
284.10	163.0
285.00	80.0

Instrument :
MSVOA_W
ClientSampleId :
BFB81