

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111422\
 Data File : VW025045.D
 Acq On : 14 Nov 2022 12:07
 Operator : SY/VA
 Sample : VW1114SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK440

Quant Time: Nov 14 23:45:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Nov 14 23:45:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	265888	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	245638	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	117422	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	50213	16.825	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.320%
7) Chloroethane-d5	2.891	69	36018	20.602	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.400%
11) 1,1-Dichloroethene-d2	4.019	63	116767	15.707	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.840%
21) 2-Butanone-d5	7.080	46	42623	42.317	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.640%
24) Chloroform-d	7.653	84	192671	23.877	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.520%
26) 1,2-Dichloroethane-d4	8.305	65	108382	23.995	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.960%
32) Benzene-d6	8.275	84	364815	23.171	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.680%
36) 1,2-Dichloropropane-d6	9.274	67	105854	22.946	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.800%
41) Toluene-d8	10.323	98	334240	22.803	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.200%
43) trans-1,3-Dichloroprop...	10.579	79	44576	21.791	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.160%
47) 2-Hexanone-d5	10.927	63	33122	41.564	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.120%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	80221	21.779	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.120%
66) 1,2-Dichlorobenzene-d4	13.853	152	109973	24.371	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.480%
Target Compounds						Qvalue
37) 1,2-Dichloropropane	9.274	63	13421	3.738	ug/L	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111422\
Data File : VW025045.D
Acq On : 14 Nov 2022 12:07
Operator : SY/VA
Sample : VW1114SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK440

Quant Time: Nov 14 23:45:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Nov 14 23:45:04 2022
Response via : Initial Calibration

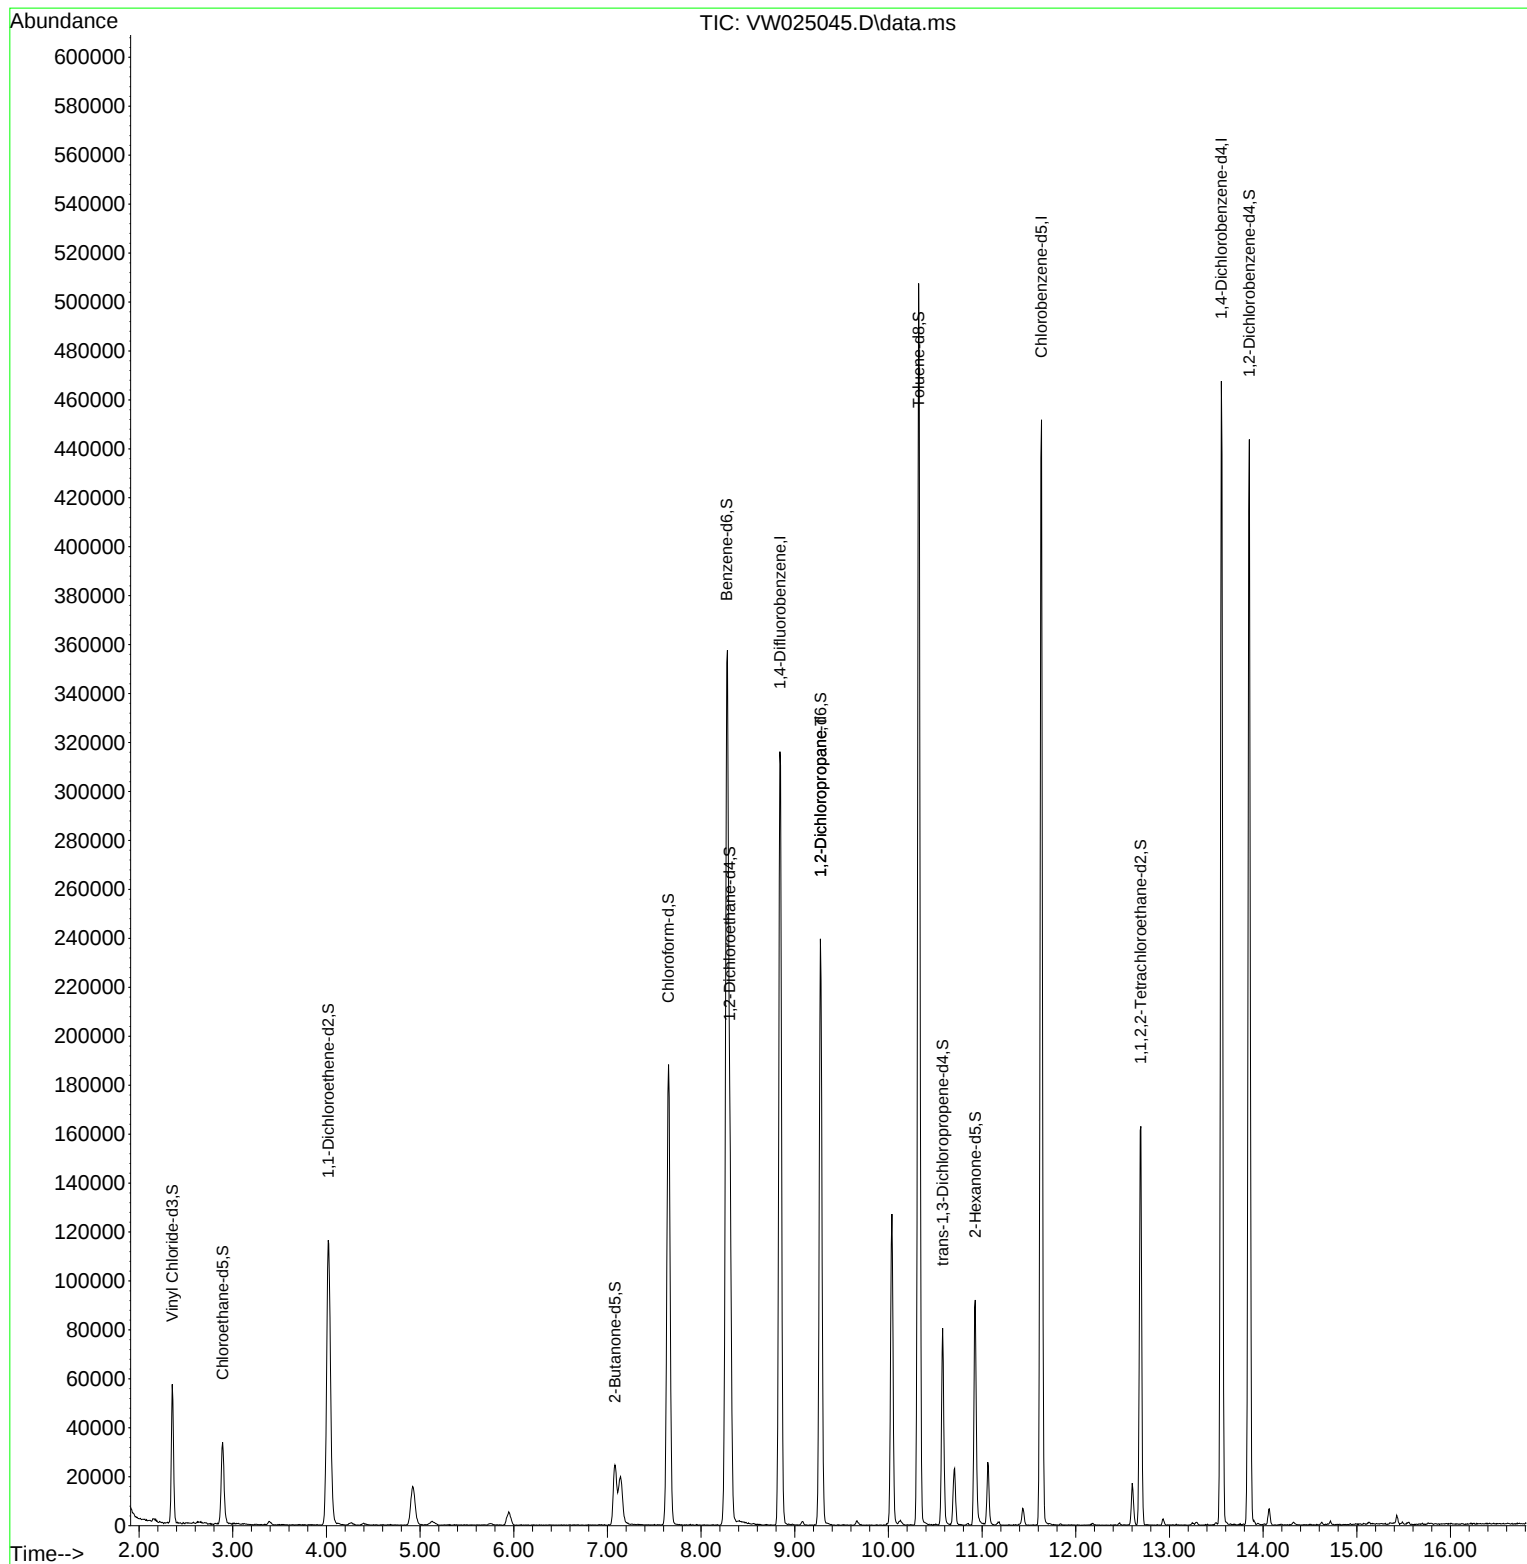

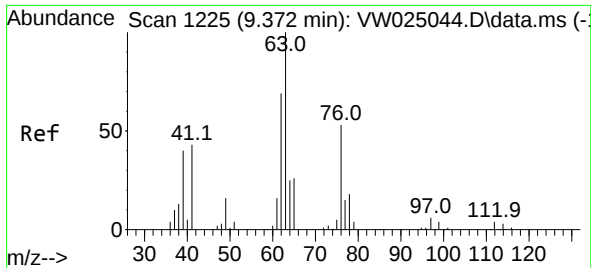

#37

1,2-Dichloropropane

Concen: 3.738 ug/L

RT: 9.274 min Scan# 11

Delta R.T. -0.098 min

Lab File: VW025045.D

Acq: 14 Nov 2022 12:07

Instrument :

MSVOA_W

ClientSampleId :

VBLK440

Tgt Ion: 63 Resp: 13421

Ion Ratio Lower Upper

63 100

112 0.0 3.6 5.4#

