
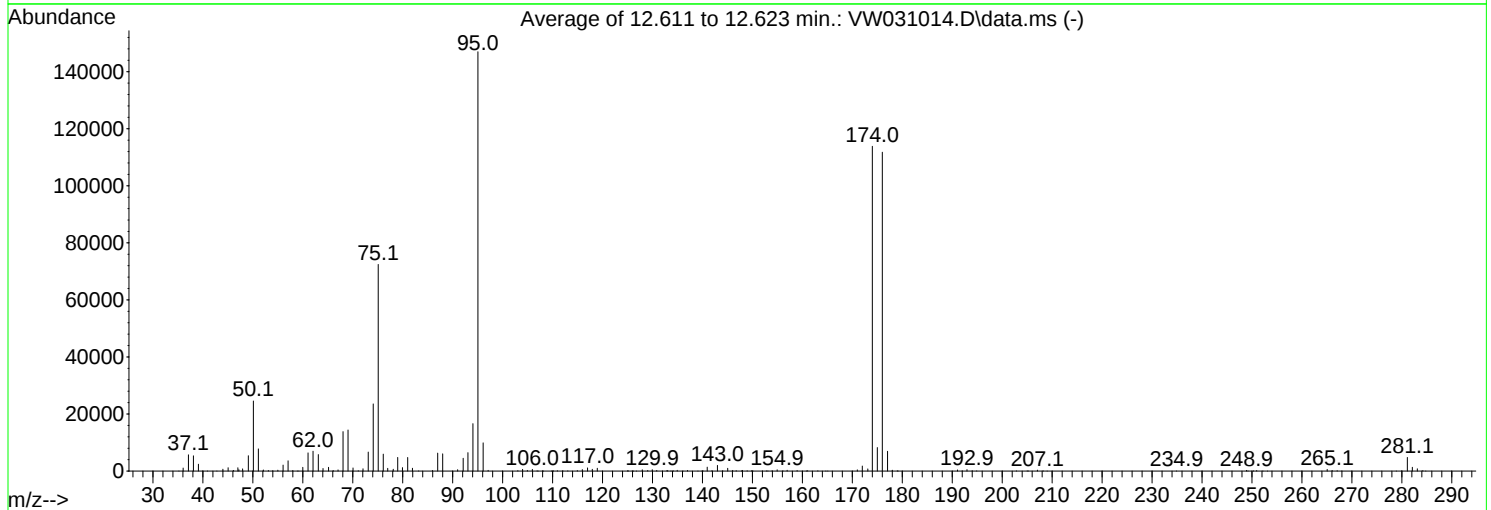


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111424\
Data File : VW031014.D
Acq On : 14 Nov 2024 08:45
Operator : SY/MD
Sample : BFB598
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB598

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Fri Nov 15 04:02:45 2024

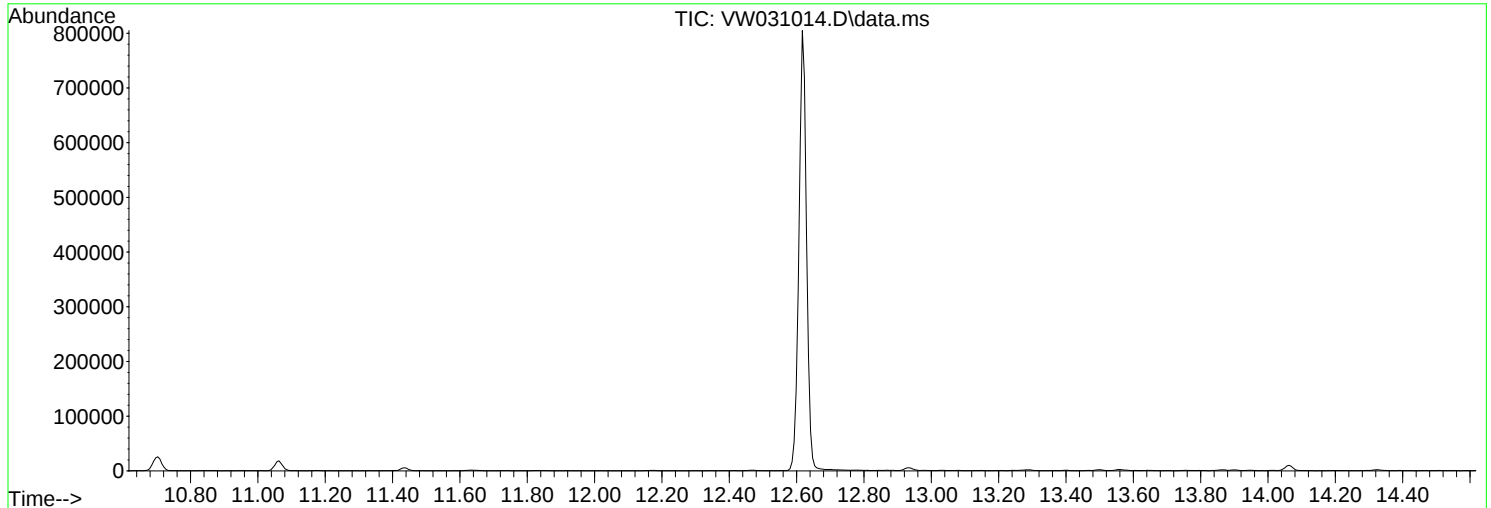

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	24565	PASS
75	95	30	80	49.3	72445	PASS
95	95	100	100	100.0	146997	PASS
96	95	5	9	6.7	9890	PASS
173	174	0.00	2	0.7	765	PASS
174	95	50	120	77.4	113845	PASS
175	174	5	9	7.2	8249	PASS
176	174	95	101	98.2	111776	PASS
177	176	5	9	6.2	6931	PASS

m/z	Abundance
36.10	63.0
38.20	62.0
40.10	211.0
44.00	158.0

Instrument :
MSVOA_W
ClientSampleId :
BFB598

m/z	Abundance
36.00	1237.0
37.10	5694.0
38.10	4921.0
39.10	1941.0
40.10	220.0
44.10	836.0
45.00	1093.0
46.20	255.0
47.00	1640.0
47.90	828.0
49.10	4688.0
50.10	21792.0
51.10	6580.0
52.10	312.0
53.20	202.0
54.00	176.0
55.00	252.0
56.00	1726.0
57.00	3131.0
58.00	71.0
60.00	1144.0
61.00	5685.0
62.00	5995.0
63.10	5659.0
64.10	799.0
65.20	1319.0
66.20	160.0
67.10	348.0
68.00	12143.0
69.10	12753.0
70.00	1103.0
71.00	94.0
72.10	771.0
73.10	6204.0
74.10	20576.0
75.10	64392.0
76.10	5141.0
77.00	809.0
78.10	479.0
79.00	4300.0
79.90	1058.0
81.00	4741.0
82.00	888.0
86.00	170.0
87.00	5327.0
88.00	4718.0
91.00	484.0
92.10	3667.0
93.00	5527.0
94.10	15063.0
95.10	129632.0
96.10	9552.0
97.10	241.0
103.00	184.0
104.00	486.0
105.00	207.0
106.10	354.0
106.90	126.0
108.00	219.0
109.80	89.0
110.10	89.0
111.00	176.0
112.00	97.0
113.00	81.0
114.90	223.0
116.00	446.0
117.00	1089.0
117.90	486.0
118.90	1089.0
125.00	334.0
126.00	165.0
128.00	413.0
129.10	209.0
129.90	387.0
130.90	155.0
132.90	669.0
133.70	147.0
135.00	300.0
137.00	145.0
139.90	85.0
140.90	1233.0
143.00	1965.0
144.10	115.0
145.10	1108.0
146.10	232.0
146.80	169.0
147.80	234.0
149.00	86.0
149.90	167.0
153.10	61.0
154.00	78.0
155.00	291.0

Instrument :
MSVOA_W
ClientSampleId :
BFB598

156.10	77.0
156.90	300.0
158.90	135.0
160.80	167.0
163.10	202.0
164.70	52.0
171.00	457.0
172.00	1576.0
174.00	80680.0
175.00	6761.0
176.00	86648.0
177.00	5976.0
178.00	301.0
179.00	320.0
191.00	633.0
192.00	149.0
193.00	817.0
194.00	142.0
194.90	142.0
202.90	62.0
205.00	176.0
207.00	507.0
208.20	145.0
209.00	71.0
234.90	101.0
248.90	404.0
250.40	105.0
250.90	332.0
253.10	65.0
265.10	970.0
266.10	296.0
267.10	266.0
268.00	52.0
280.00	170.0
281.10	6644.0
282.10	2242.0
283.10	1113.0
284.20	263.0
284.80	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB598

m/z	Abundance
36.10	1078.0
37.10	6315.0
38.10	6244.0
39.10	2998.0
39.90	286.0
42.80	79.0
44.10	895.0
45.10	1399.0
46.10	239.0
47.00	1886.0
48.00	745.0
49.10	6198.0
50.10	28704.0
51.10	9274.0
52.20	469.0
53.10	237.0
54.10	104.0
55.00	392.0
56.10	2641.0
57.00	4194.0
58.00	210.0
58.90	132.0
60.00	1507.0
61.10	7102.0
62.10	8323.0
63.10	6322.0
64.10	1196.0
65.10	1417.0
66.00	150.0
67.00	469.0
68.10	15581.0
69.00	15831.0
70.10	1155.0
71.10	138.0
72.00	741.0
73.10	7581.0
74.10	26632.0
75.10	81616.0
76.10	6430.0
77.00	996.0
78.10	758.0
79.00	5595.0
80.00	1467.0
81.00	5380.0
82.00	1208.0
83.20	77.0
86.00	217.0
87.00	7019.0
88.00	7295.0
91.00	577.0
92.10	5200.0
93.10	7429.0
94.00	18272.0
95.10	164352.0
96.10	10496.0
97.00	298.0
103.10	189.0
104.00	744.0
104.90	260.0
105.90	733.0
107.10	78.0
108.20	76.0
110.10	152.0
110.90	118.0
112.00	197.0
113.00	86.0
115.00	215.0
115.90	616.0
117.00	1245.0
118.00	808.0
119.00	931.0
125.20	188.0
126.20	61.0
127.90	548.0
129.00	283.0
130.00	623.0
130.80	248.0
132.00	51.0
133.10	322.0
134.20	153.0
134.90	309.0
137.00	240.0
140.10	198.0
141.00	1587.0
141.90	273.0
143.00	2108.0
144.10	116.0
145.00	1094.0
146.00	261.0
146.70	203.0
148.00	311.0
148.90	177.0

Instrument :
MSVOA_W
ClientSampleId :
BFB598

149.80	175.0
152.10	60.0
152.80	198.0
153.90	96.0
154.90	565.0
156.10	81.0
156.90	321.0
159.00	244.0
161.10	188.0
163.10	90.0
171.00	545.0
172.10	2095.0
173.10	2294.0
174.00	129336.0
175.00	9694.0
176.00	131072.0
177.10	7083.0
178.00	328.0
179.20	66.0
191.10	433.0
192.00	116.0
192.90	534.0
194.00	100.0
194.90	69.0
202.80	77.0
205.20	161.0
207.10	373.0
208.20	61.0
248.90	295.0
250.20	107.0
251.00	150.0
265.00	551.0
266.10	194.0
266.90	143.0
278.90	72.0
279.90	55.0
281.10	5361.0
282.10	1212.0
283.10	744.0
284.20	155.0

Instrument :
MSVOA_W
ClientSampleId :
BFB598

m/z	Abundance
35.20	50.0
36.00	1054.0
37.10	5113.0
38.10	5053.0
39.10	2262.0
40.00	211.0
40.90	126.0
44.00	742.0
45.10	1037.0
46.20	209.0
47.20	1399.0
48.00	771.0
49.10	5272.0
50.10	23200.0
51.10	7459.0
52.00	373.0
53.00	175.0
53.90	113.0
55.00	336.0
56.00	1988.0
57.10	3507.0
58.00	300.0
59.20	52.0
60.00	1288.0
61.10	6364.0
62.10	6597.0
63.10	5411.0
64.00	758.0
65.10	1235.0
66.10	182.0
67.10	459.0
68.10	13785.0
69.10	14628.0
70.00	1005.0
71.20	113.0
72.00	887.0
73.10	6224.0
74.10	23432.0
75.10	71328.0
76.10	6244.0
77.00	1103.0
78.10	664.0
79.00	4445.0
79.90	1141.0
81.00	4200.0
81.90	906.0
83.20	69.0
85.80	188.0
87.00	6546.0
88.00	6124.0
91.00	440.0
92.10	4638.0
93.10	6417.0
94.00	16576.0
95.00	147008.0
96.10	9622.0
97.20	208.0
103.00	163.0
104.00	538.0
104.90	244.0
106.00	704.0
106.90	151.0
108.00	58.0
110.20	88.0
111.00	96.0
112.10	114.0
113.10	112.0
114.90	136.0
116.00	513.0
117.00	1000.0
118.00	557.0
118.90	968.0
125.10	123.0
125.80	74.0
126.80	71.0
127.90	384.0
129.00	192.0
129.90	455.0
130.90	269.0
133.00	220.0
134.10	90.0
135.00	215.0
136.10	61.0
137.00	309.0
139.10	87.0
140.10	104.0
141.00	1339.0
141.80	64.0
143.00	1896.0
144.00	146.0
145.00	743.0
146.10	236.0

Instrument :
MSVOA_W
ClientSampleId :
BFB598

146.70	101.0
148.00	410.0
148.90	116.0
150.10	162.0
151.90	91.0
153.10	109.0
154.00	122.0
154.90	505.0
156.10	87.0
157.00	246.0
159.00	247.0
161.00	232.0
165.10	54.0
171.00	326.0
171.90	1617.0
174.00	131520.0
175.00	8292.0
176.00	117608.0
177.00	7733.0
178.00	267.0
179.10	70.0
191.00	166.0
193.10	239.0
194.00	56.0
202.90	54.0
207.10	171.0
249.20	190.0
250.90	95.0
252.20	60.0
265.10	245.0
265.90	102.0
267.20	52.0
281.10	2323.0
282.20	551.0
283.10	542.0
284.10	123.0

Instrument :
MSVOA_W
ClientSampleId :
BFB598