

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
 Data File : VW017230.D
 Acq On : 15 Nov 2020 12:08
 Operator : SY/VA
 Sample : L4727-11
 Misc : 3.80G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:52:30 PM

Quant Time: Nov 16 10:00:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 09:47:42 2020
 Response via : Initial Calibration

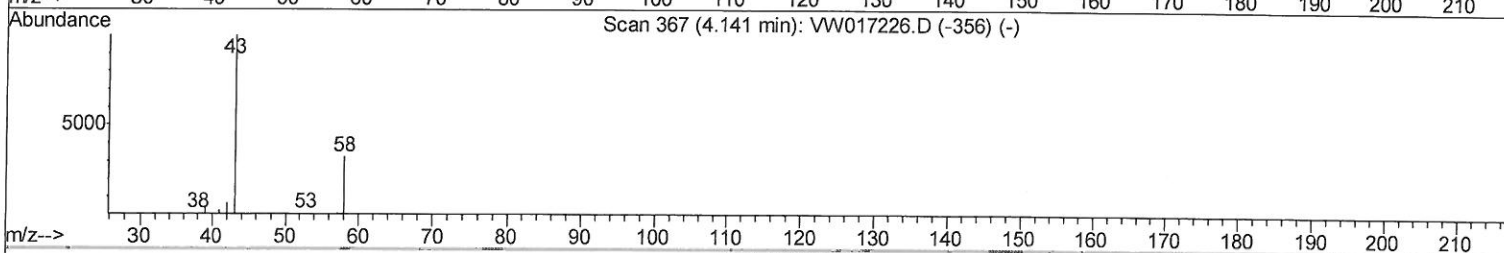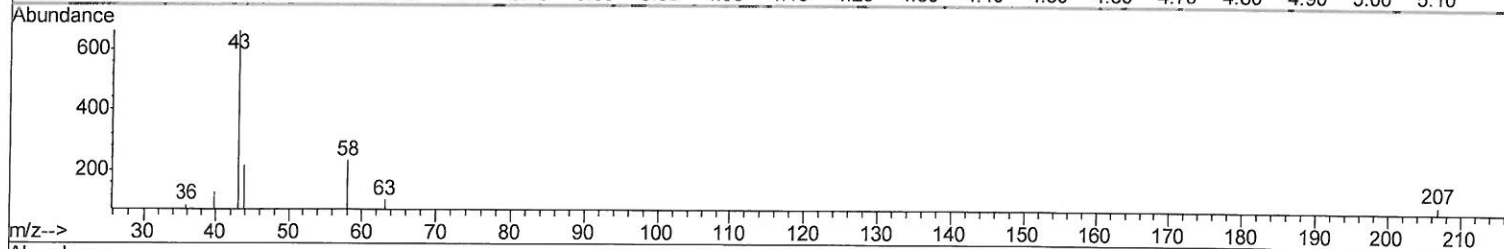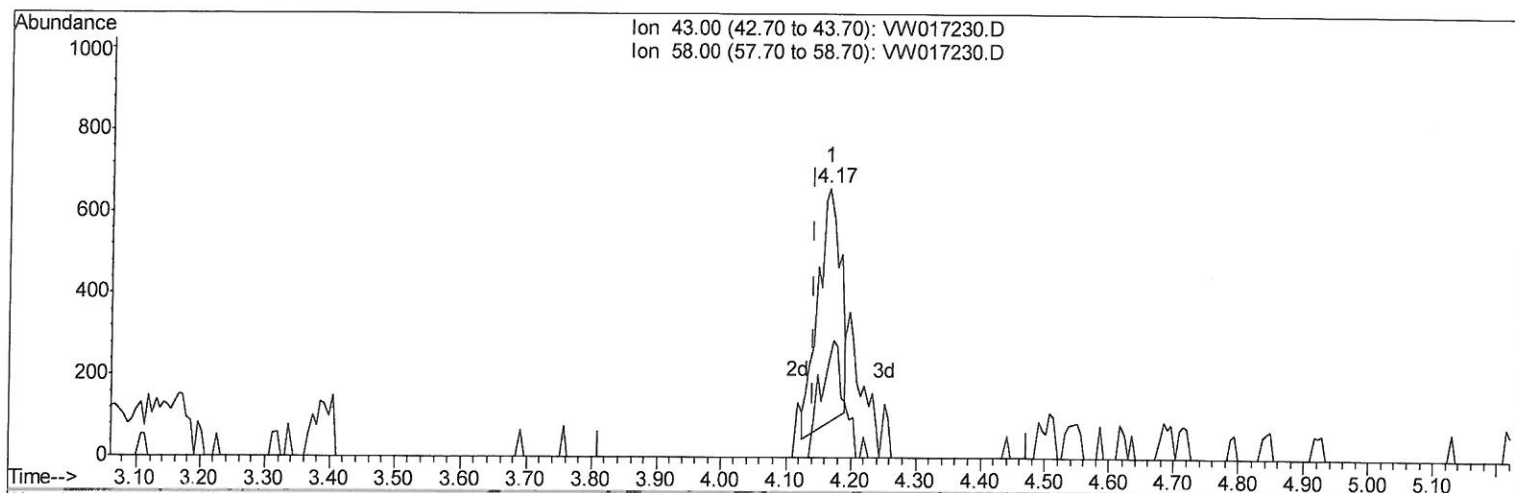

TIC: VW017230.D

(13) Acetone (T)

4.166min (+0.024) 1.64ug/L

response 1393

Ion	Exp%	Act%
43.00	100	100
58.00	34.60	38.33
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
 Data File : VW017230.D
 Acq On : 15 Nov 2020 12:08
 Operator : SY/VA
 Sample : L4727-11
 Misc : 3.80G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:52:30 PM

Quant Time: Nov 16 10:00:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 09:47:42 2020
 Response via : Initial Calibration

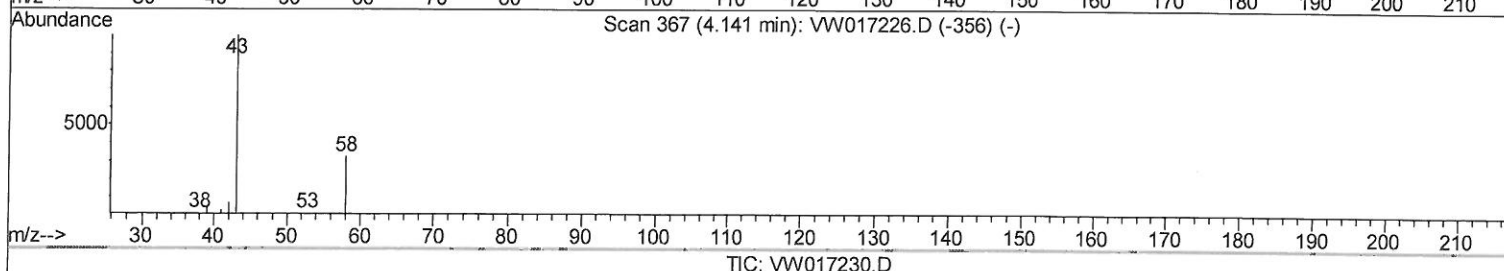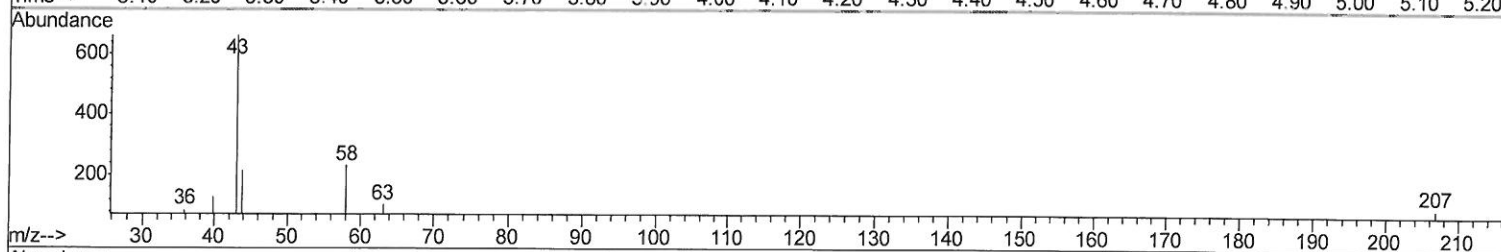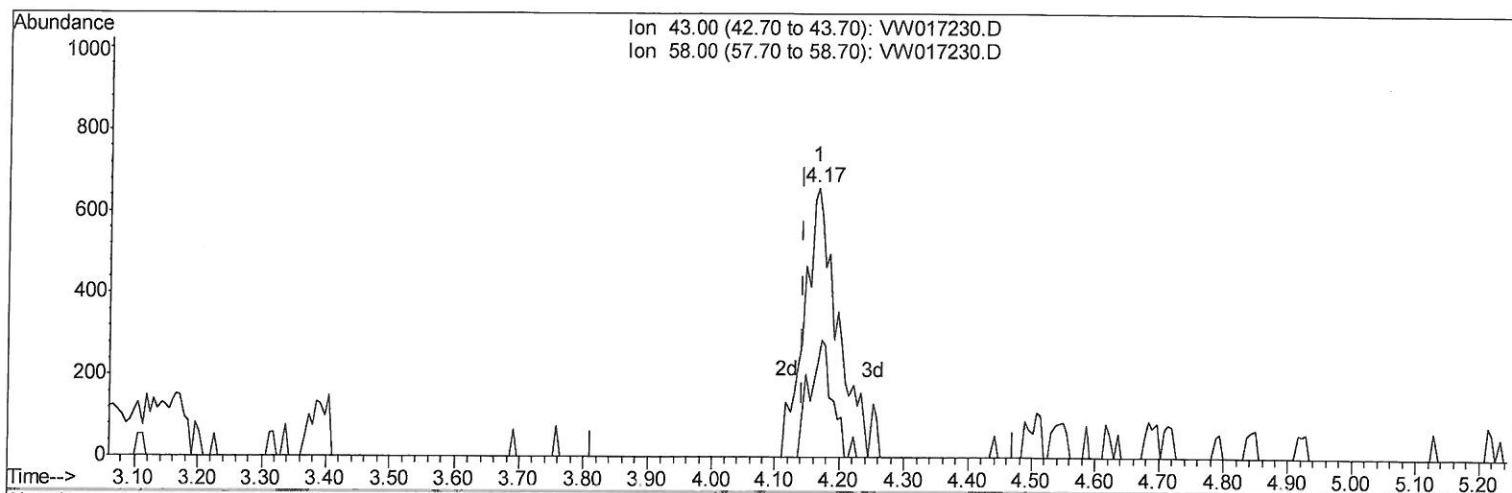

(13) Acetone (T)

4.166min (+0.024) 2.77ug/L m

> 11/18/2024

response 2350

Ion	Exp%	Act%
43.00	100	100
58.00	34.60	22.72
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
 Data File : VW017230.D
 Acq On : 15 Nov 2020 12:08
 Operator : SY/VA
 Sample : L4727-11
 Misc : 3.80G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:52:30 PM

Quant Time: Nov 16 10:07:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 09:47:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	449225	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	375100	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	148312	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	118383	20.92	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.68%		
7) Chloroethane-d5	2.89	69	102902	23.60	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	94.40%		
10) 1,1-Dichloroethene-d2	4.02	63	163526	16.16	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.64%		
20) 2-Butanone-d5	7.09	46	41770	33.01	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	66.02%		
24) Chloroform-d	7.65	84	245506	23.41	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.64%		
26) 1,2-Dichloroethane-d4	8.31	65	119387	22.90	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.60%		
29) Benzene-d6	8.28	84	482003	25.23	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	100.92%		
33) 1,2-Dichloropropane-d6	9.28	67	133761	25.32	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.28%		
37) Toluene-d8	10.33	98	436425	24.23	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	96.92%		
38) trans-1,3-Dichloropropene-	10.58	79	49490	20.78	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.12%		
39) 2-Hexanone-d5	10.93	63	34373	37.28	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	74.56%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	95381	20.72	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	82.88%		
61) 1,2-Dichlorobenzene-d4	13.86	152	128960	24.68	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.72%		

Target Compounds

13) Acetone	4.17	43	2350m)	2.774	ug/L	Ovalue
16) Methylene chloride	4.93	84	11194	1.848	ug/L	11/18/2020 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
Data File : VW017230.D
Acq On : 15 Nov 2020 12:08
Operator : SY/VA
Sample : L4727-11
Misc : 3.80G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0AC6

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:52:30 PM

Quant Time: Nov 16 10:07:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 16 09:47:42 2020
Response via : Initial Calibration

