

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
 Data File : VW017241.D
 Acq On : 15 Nov 2020 16:26
 Operator : SY/VA
 Sample : L4739-02
 Misc : 5.61G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 GB0Z1

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:52:41 PM

Quant Time: Nov 16 12:33:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

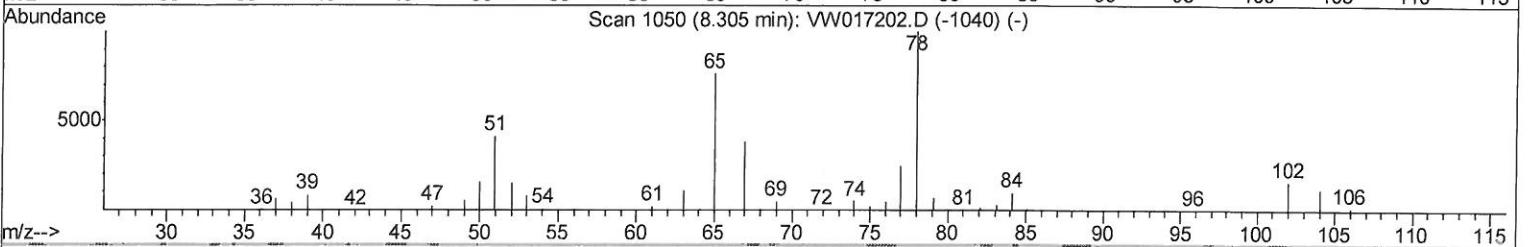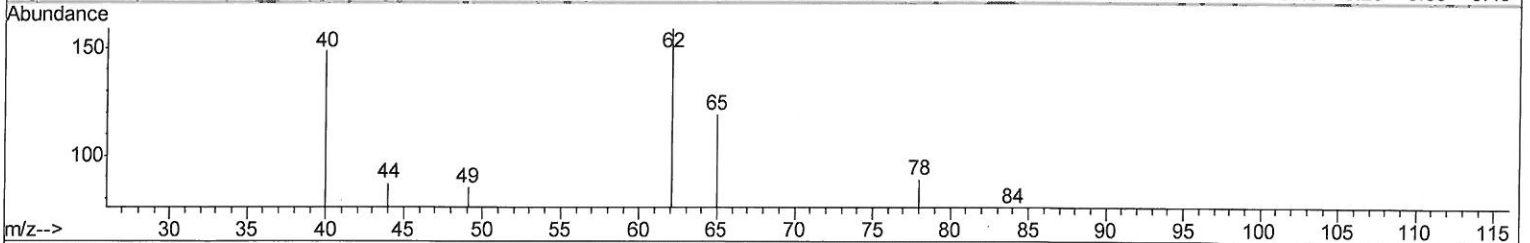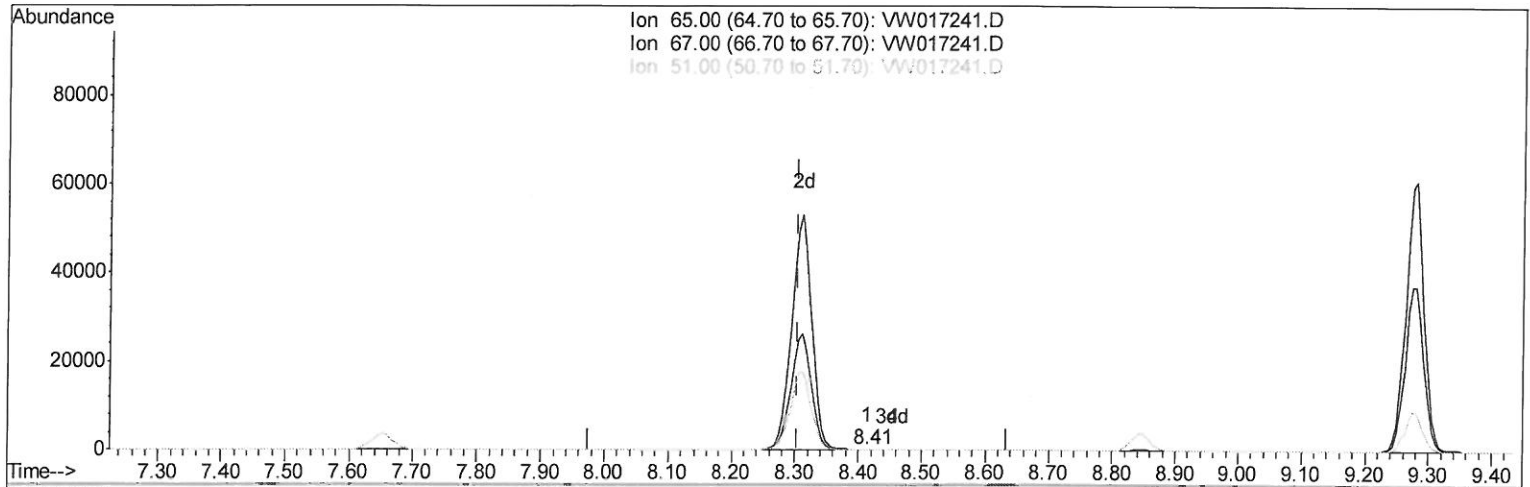

TIC: VW017241.D

(26) 1,2-Dichloroethane-d4 (S)

8.415min (+0.110) 0.02ug/L

response 106

Ion	Exp%	Act%
65.00	100	100
67.00	53.70	65.09
51.00	92.10	78.30
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111520\
 Data File : VW017241.D
 Acq On : 15 Nov 2020 16:26
 Operator : SY/VA
 Sample : L4739-02
 Misc : 5.61G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 GB0Z1

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:52:41 PM

Quant Time: Nov 16 14:43:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

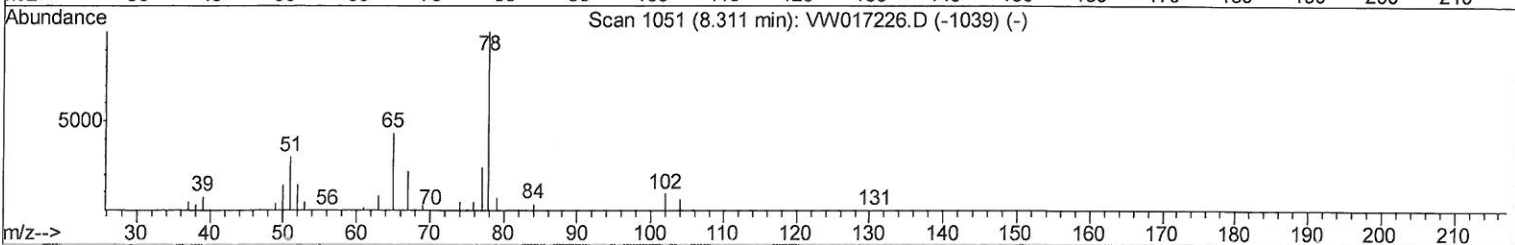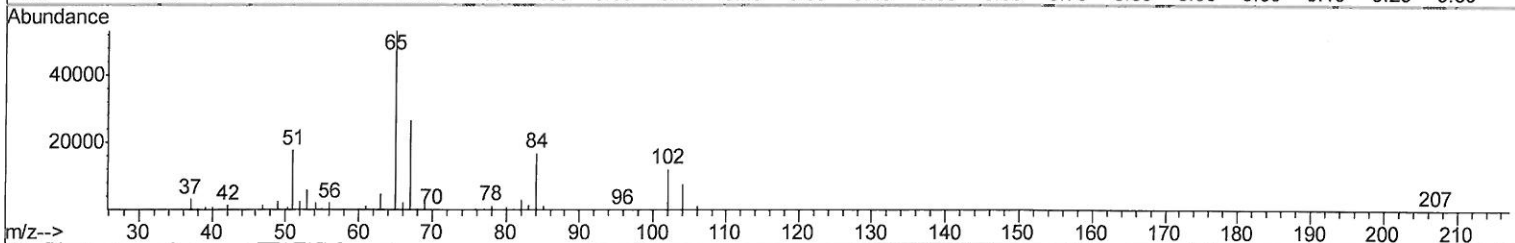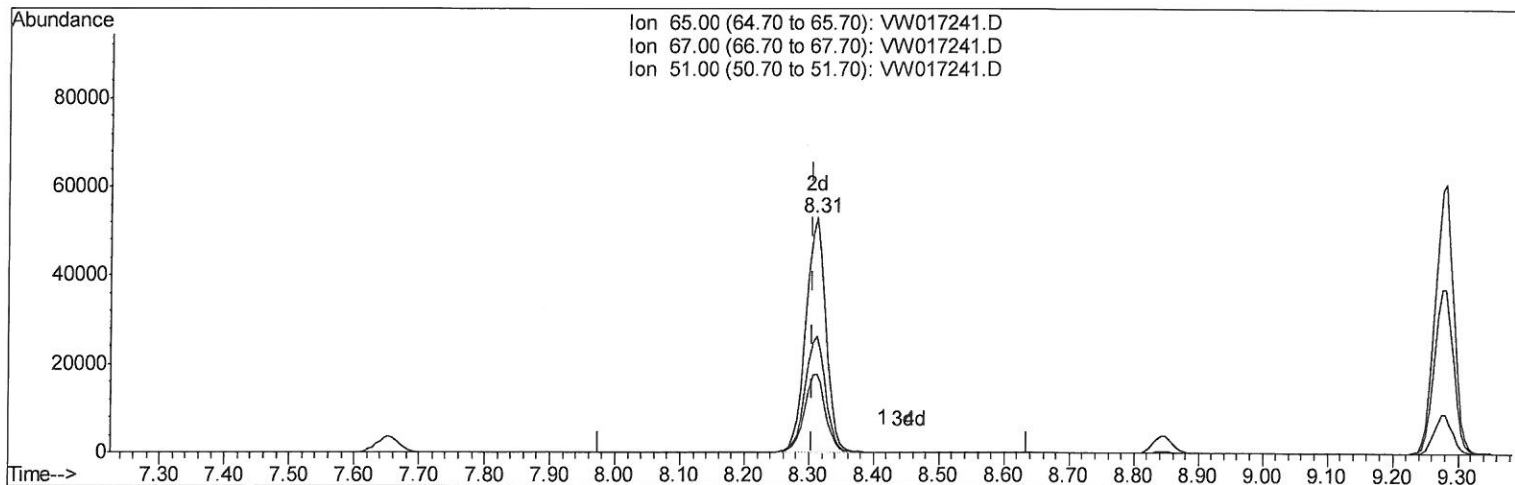

TIC: VW017241.D

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+0.006) 21.51ug/L m

response 115417

Ion	Exp%	Act%
65.00	100	100
67.00	53.70	0.06#
51.00	92.10	0.07#
0.00	0.00	0.00

11/30/2027

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\WV111520\
 Data File : VW017241.D
 Acq On : 15 Nov 2020 16:26
 Operator : SY/VA
 Sample : L4739-02
 Misc : 5.61G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB0Z1

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:52:41 PM

Quant Time: Nov 16 14:43:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	462304	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	402458	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	167363	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	93956	16.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.56%
7) Chloroethane-d5	2.90	69	83800	18.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.72%
10) 1,1-Dichloroethene-d2	4.02	63	148066	14.22	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.88%
20) 2-Butanone-d5	7.09	46	46152	35.44	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.88%
24) Chloroform-d	7.65	84	222608	20.63	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.52%
26) 1,2-Dichloroethane-d4	8.31	65	115417m	21.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.04%
29) Benzene-d6	8.28	84	431758	21.07	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.28%
33) 1,2-Dichloropropane-d6	9.28	67	120232	21.21	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.84%
37) Toluene-d8	10.33	98	420876	21.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.12%
38) trans-1,3-Dichloropropene-	10.58	79	51295	20.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.28%
39) 2-Hexanone-d5	10.93	63	40229	40.66	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.32%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	98919	20.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.12%
61) 1,2-Dichlorobenzene-d4	13.85	152	123625	20.97	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.88%

Target Compounds					Ovalue
13) Acetone	4.13	43	14131	16.207	ug/L 97
44) Toluene	10.39	91	9994	0.430	ug/L 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
Data File : VW017241.D
Acq On : 15 Nov 2020 16:26
Operator : SY/VA
Sample : L4739-02
Misc : 5.61G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GB0Z1

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:52:41 PM

Quant Time: Nov 16 12:50:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 16 11:48:24 2020
Response via : Initial Calibration

