

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
 Data File : VW017243.D
 Acq On : 15 Nov 2020 17:13
 Operator : SY/VA
 Sample : L4710-10
 Misc : 4.60G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 C0BF0

Manual Integrations
APPROVED

MMDadoda
 11/17/2020 6:52:43 PM

Quant Time: Nov 16 12:33:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

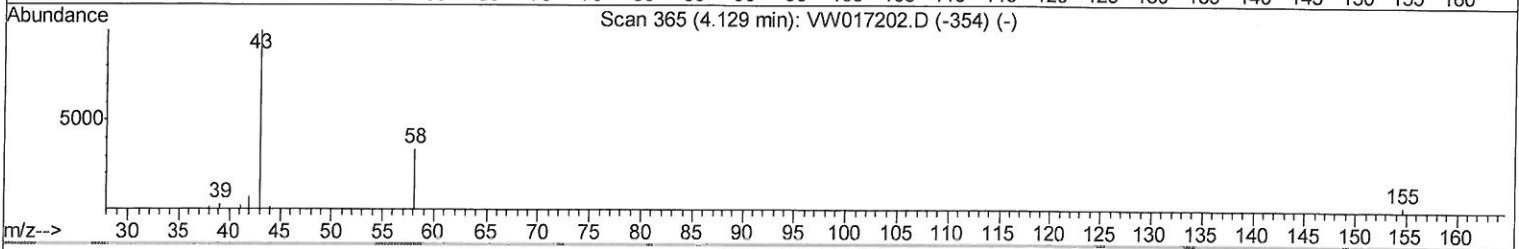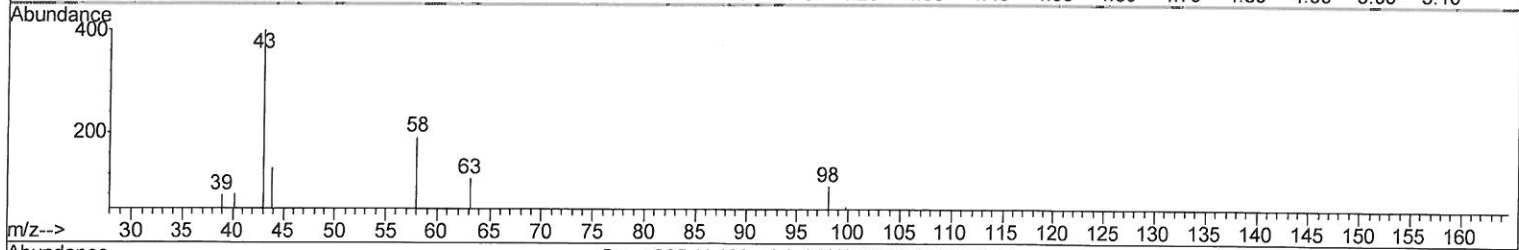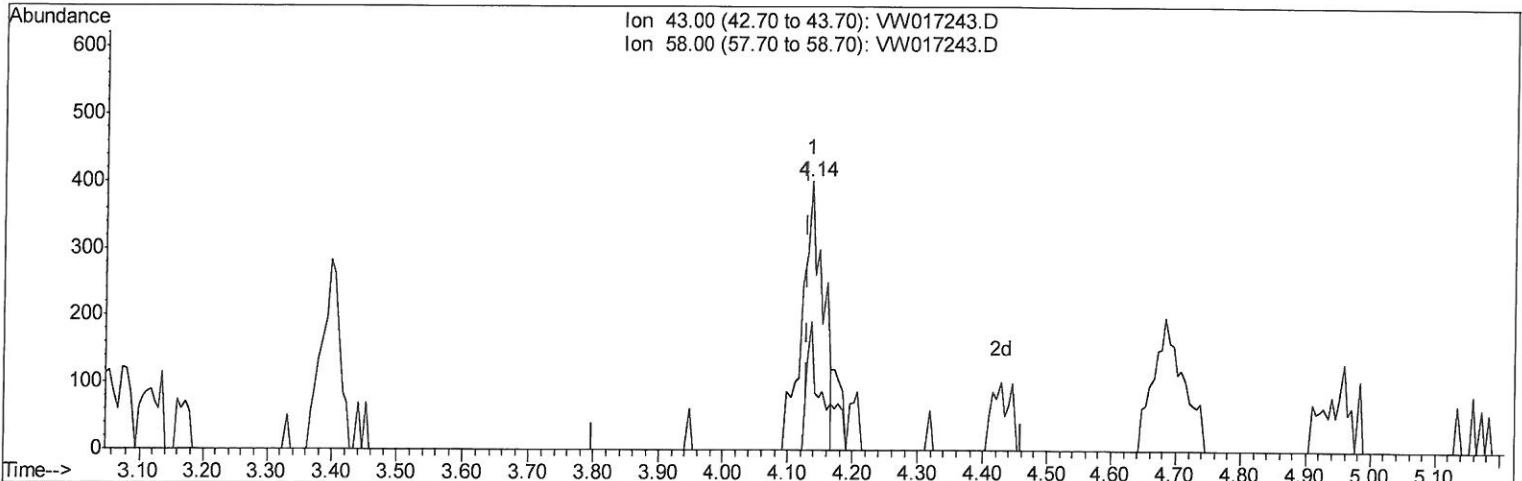

TIC: VW017243.D

(13) Acetone (T)

4.135min (+0.006) 1.34ug/L

response 891

Ion	Exp%	Act%
43.00	100	100
58.00	34.60	20.20
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
 Data File : VW017243.D
 Acq On : 15 Nov 2020 17:13
 Operator : SY/VA
 Sample : L4710-10
 Misc : 4.60G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BF0

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:52:43 PM

Quant Time: Nov 16 12:33:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

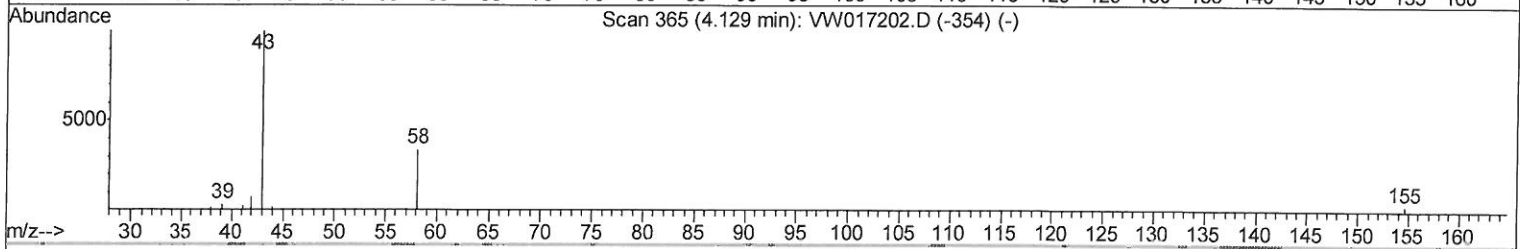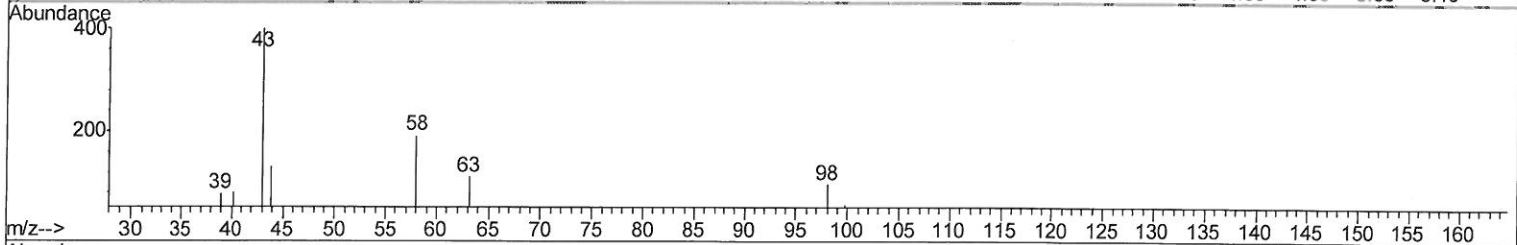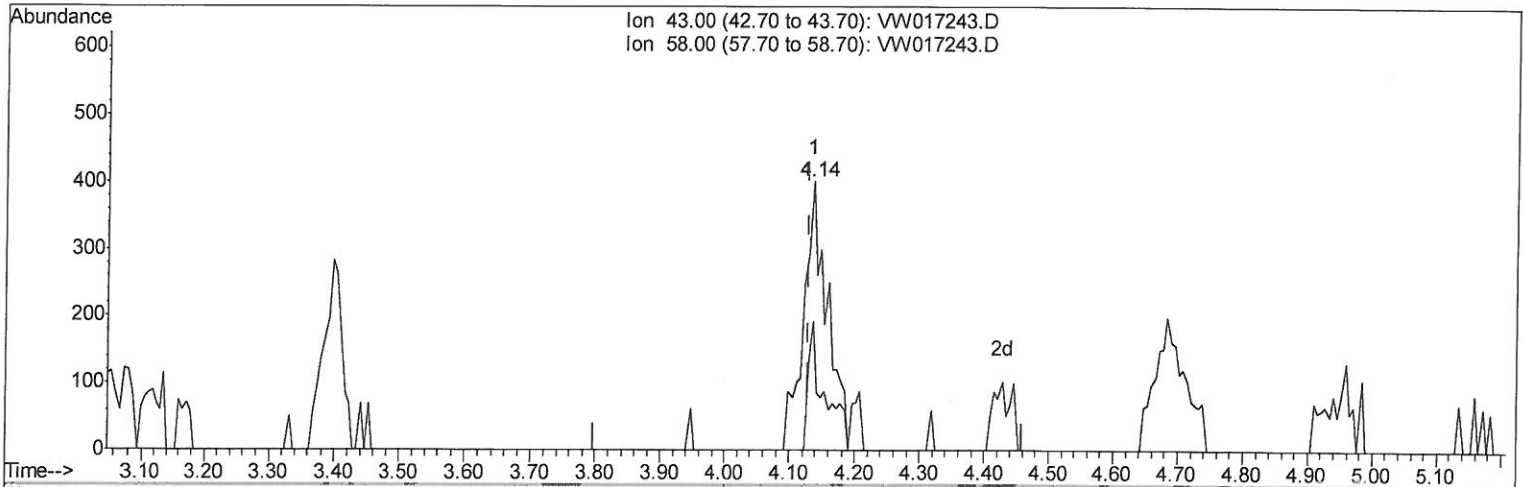

TIC: VW017243.D

(13) Acetone (T)

4.135min (+0.006) 1.51ug/L m

11/18/2020

response 1006

Ion	Exp%	Act%
43.00	100	100
58.00	34.60	17.89
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
 Data File : VW017243.D
 Acq On : 15 Nov 2020 17:13
 Operator : SY/VA
 Sample : L4710-10
 Misc : 4.60G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BF0

Manual Integrations
 APPROVED

MMDadoda
 11/17/2020 6:52:43 PM

Quant Time: Nov 16 12:56:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Nov 16 11:48:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	352120	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	253833	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	82391	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.35	65	83384	18.80	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.20%		
7) Chloroethane-d5	2.90	69	74626	21.83	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.32%		
10) 1,1-Dichloroethene-d2	4.02	63	123909	15.62	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.48%		
20) 2-Butanone-d5	7.09	46	24737	24.94	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	49.88%		
24) Chloroform-d	7.65	84	185578	22.58	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.32%		
26) 1,2-Dichloroethane-d4	8.31	65	97140	23.77	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.08%		
29) Benzene-d6	8.28	84	346903	26.84	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	107.36%		
33) 1,2-Dichloropropane-d6	9.28	67	98172	27.46	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	109.84%		
37) Toluene-d8	10.33	98	294570	24.17	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	96.68%		
38) trans-1,3-Dichloropropene-	10.58	79	32013	19.86	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.44%		
39) 2-Hexanone-d5	10.93	63	18414	29.51	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	59.02%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	61636	19.79	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	79.16%		
61) 1,2-Dichlorobenzene-d4	13.86	152	65165	22.45	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.80%		
Target Compounds						
13) Acetone	4.14	43	1006m	1.515	ug/L	Ovalue
16) Methylene chloride	4.92	84	9033	1.903	ug/L	11/18/2020 5:24 PM

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111520\
Data File : VW017243.D
Acq On : 15 Nov 2020 17:13
Operator : SY/VA
Sample : L4710-10
Misc : 4.60G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BF0

Manual Integrations
APPROVED

MMDadoda
11/17/2020 6:52:43 PM

Quant Time: Nov 16 12:56:56 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Mon Nov 16 11:48:24 2020
Response via : Initial Calibration

