

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111522\
 Data File : VW025051.D
 Acq On : 15 Nov 2022 10:18
 Operator : SY/VA
 Sample : VW1115SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK441

Quant Time: Nov 16 00:12:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 16 00:12:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	290391	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	261737	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	126769	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	52825	16.207	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.840%
7) Chloroethane-d5	2.891	69	38304	20.061	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.240%
11) 1,1-Dichloroethene-d2	4.025	63	122425	15.078	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.320%
21) 2-Butanone-d5	7.086	46	44274	40.247	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.500%
24) Chloroform-d	7.653	84	201640	22.880	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.520%
26) 1,2-Dichloroethane-d4	8.305	65	112258	22.756	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.040%
32) Benzene-d6	8.274	84	382230	22.784	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.120%
36) 1,2-Dichloropropane-d6	9.274	67	110551	22.490	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.960%
41) Toluene-d8	10.323	98	350594	22.447	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.800%
43) trans-1,3-Dichloroprop...	10.579	79	47138	21.626	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.520%
47) 2-Hexanone-d5	10.926	63	35440	41.737	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.480%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	85612	21.813	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	116193	23.851	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.400%
Target Compounds						Qvalue
34) Trichloroethene	8.847	95	9467	2.269	ug/L #	7
37) 1,2-Dichloropropane	9.274	63	14012	3.663	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111522\
Data File : VW025051.D
Acq On : 15 Nov 2022 10:18
Operator : SY/VA
Sample : VW1115SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK441

Quant Time: Nov 16 00:12:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 16 00:12:11 2022
Response via : Initial Calibration




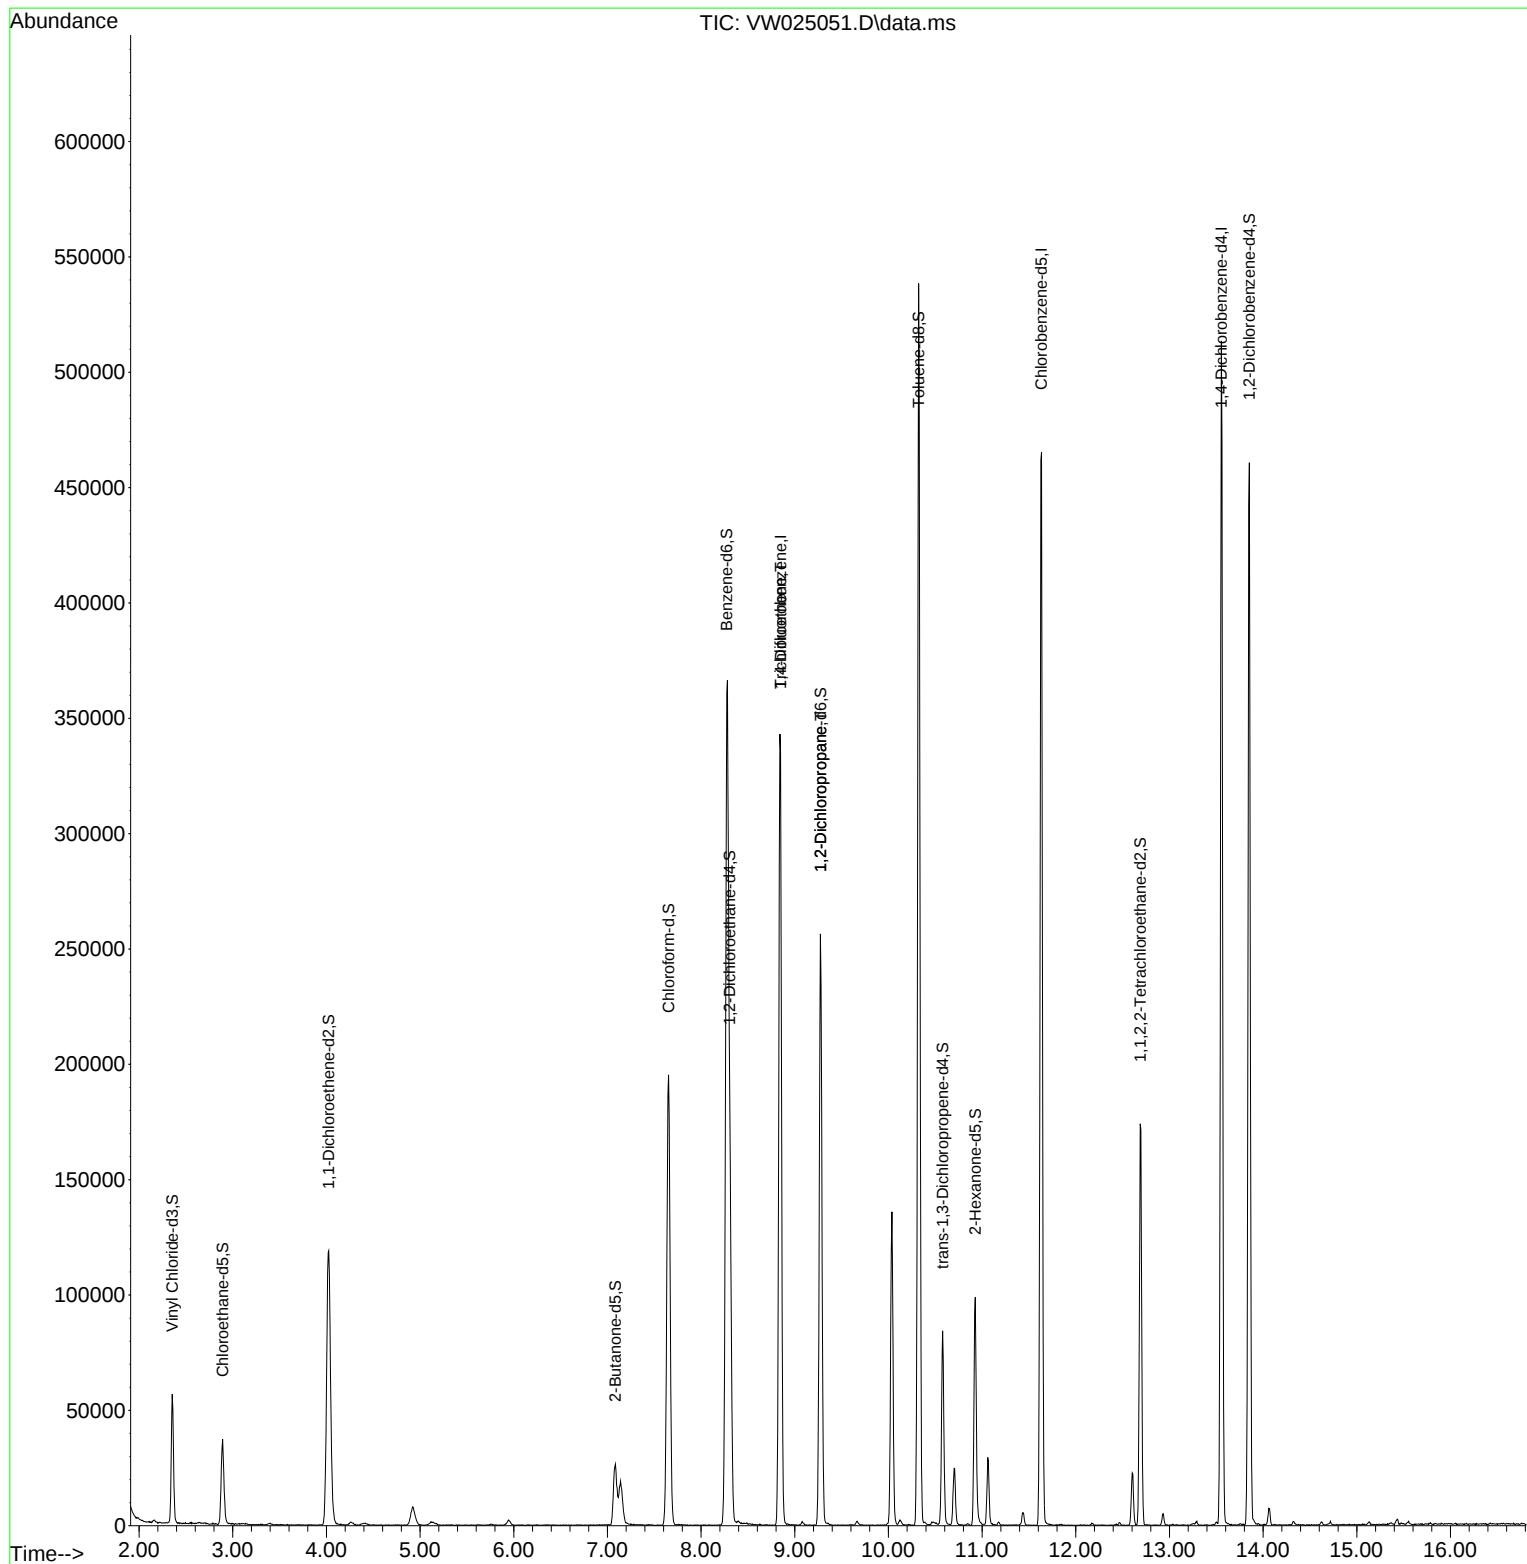


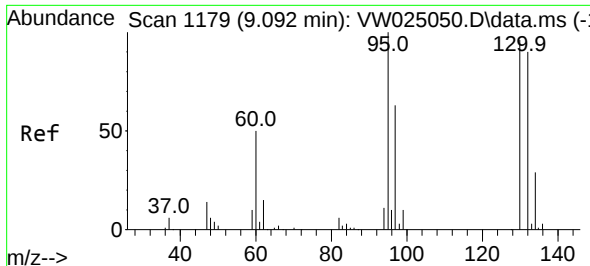

#34
 Trichloroethene
 Concen: 2.269 ug/L
 RT: 8.847 min Scan# 1179
 Delta R.T. -0.244 min
 Lab File: VW025051.D
 Acq: 15 Nov 2022 10:18

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK441

Tgt Ion: 95	Resp: 9467
Ion Ratio	Lower Upper
95	100
97	0.0 44.7 83.1#
132	0.0 62.6 116.2#
130	0.0 69.1 128.3#

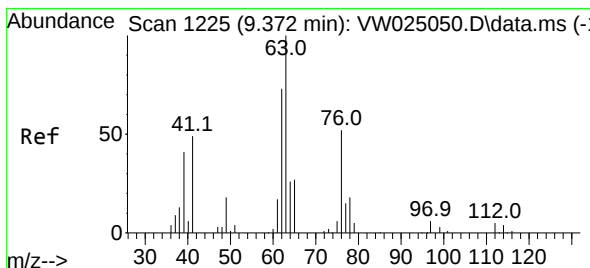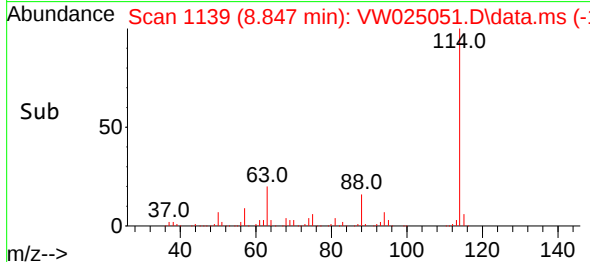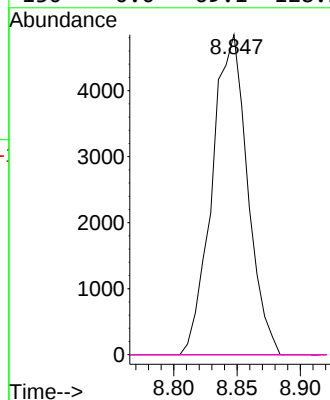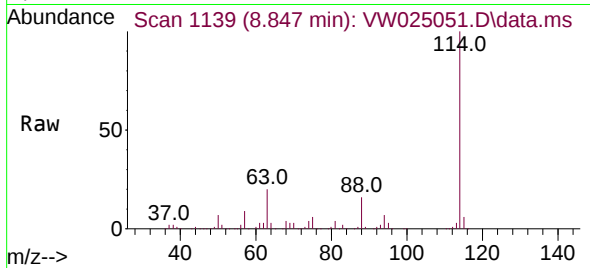

#37
 1,2-Dichloropropane
 Concen: 3.663 ug/L
 RT: 9.274 min Scan# 1209
 Delta R.T. -0.098 min
 Lab File: VW025051.D
 Acq: 15 Nov 2022 10:18

Tgt Ion: 63	Resp: 14012
Ion Ratio	Lower Upper
63	100
112	0.0 3.6 5.4#

