

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111522\
 Data File : VW025052.D
 Acq On : 15 Nov 2022 11:05
 Operator : SY/VA
 Sample : N5603-07
 Misc : 5.10g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Nov 16 00:12:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Nov 16 00:12:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	326767	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	302796	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	154769	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	55321	15.083	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.320%
7) Chloroethane-d5	2.891	69	40960	19.064	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.240%
11) 1,1-Dichloroethene-d2	4.019	63	132199	14.470	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.880%
21) 2-Butanone-d5	7.073	46	61158	49.406	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.820%
24) Chloroform-d	7.653	84	218928	22.076	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.320%
26) 1,2-Dichloroethane-d4	8.305	65	127736	23.011	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.040%
32) Benzene-d6	8.274	84	407614	21.002	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.000%
36) 1,2-Dichloropropane-d6	9.274	67	122241	21.496	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.000%
41) Toluene-d8	10.323	98	378398	20.942	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.760%
43) trans-1,3-Dichloroprop...	10.579	79	55196	21.889	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.560%
47) 2-Hexanone-d5	10.920	63	49416	50.305	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.600%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	108132	23.814	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	132831	22.333	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.320%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	28027	4.831	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111522\
Data File : VW025052.D
Acq On : 15 Nov 2022 11:05
Operator : SY/VA
Sample : N5603-07
Misc : 5.10g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Nov 16 00:12:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Nov 16 00:12:11 2022
Response via : Initial Calibration

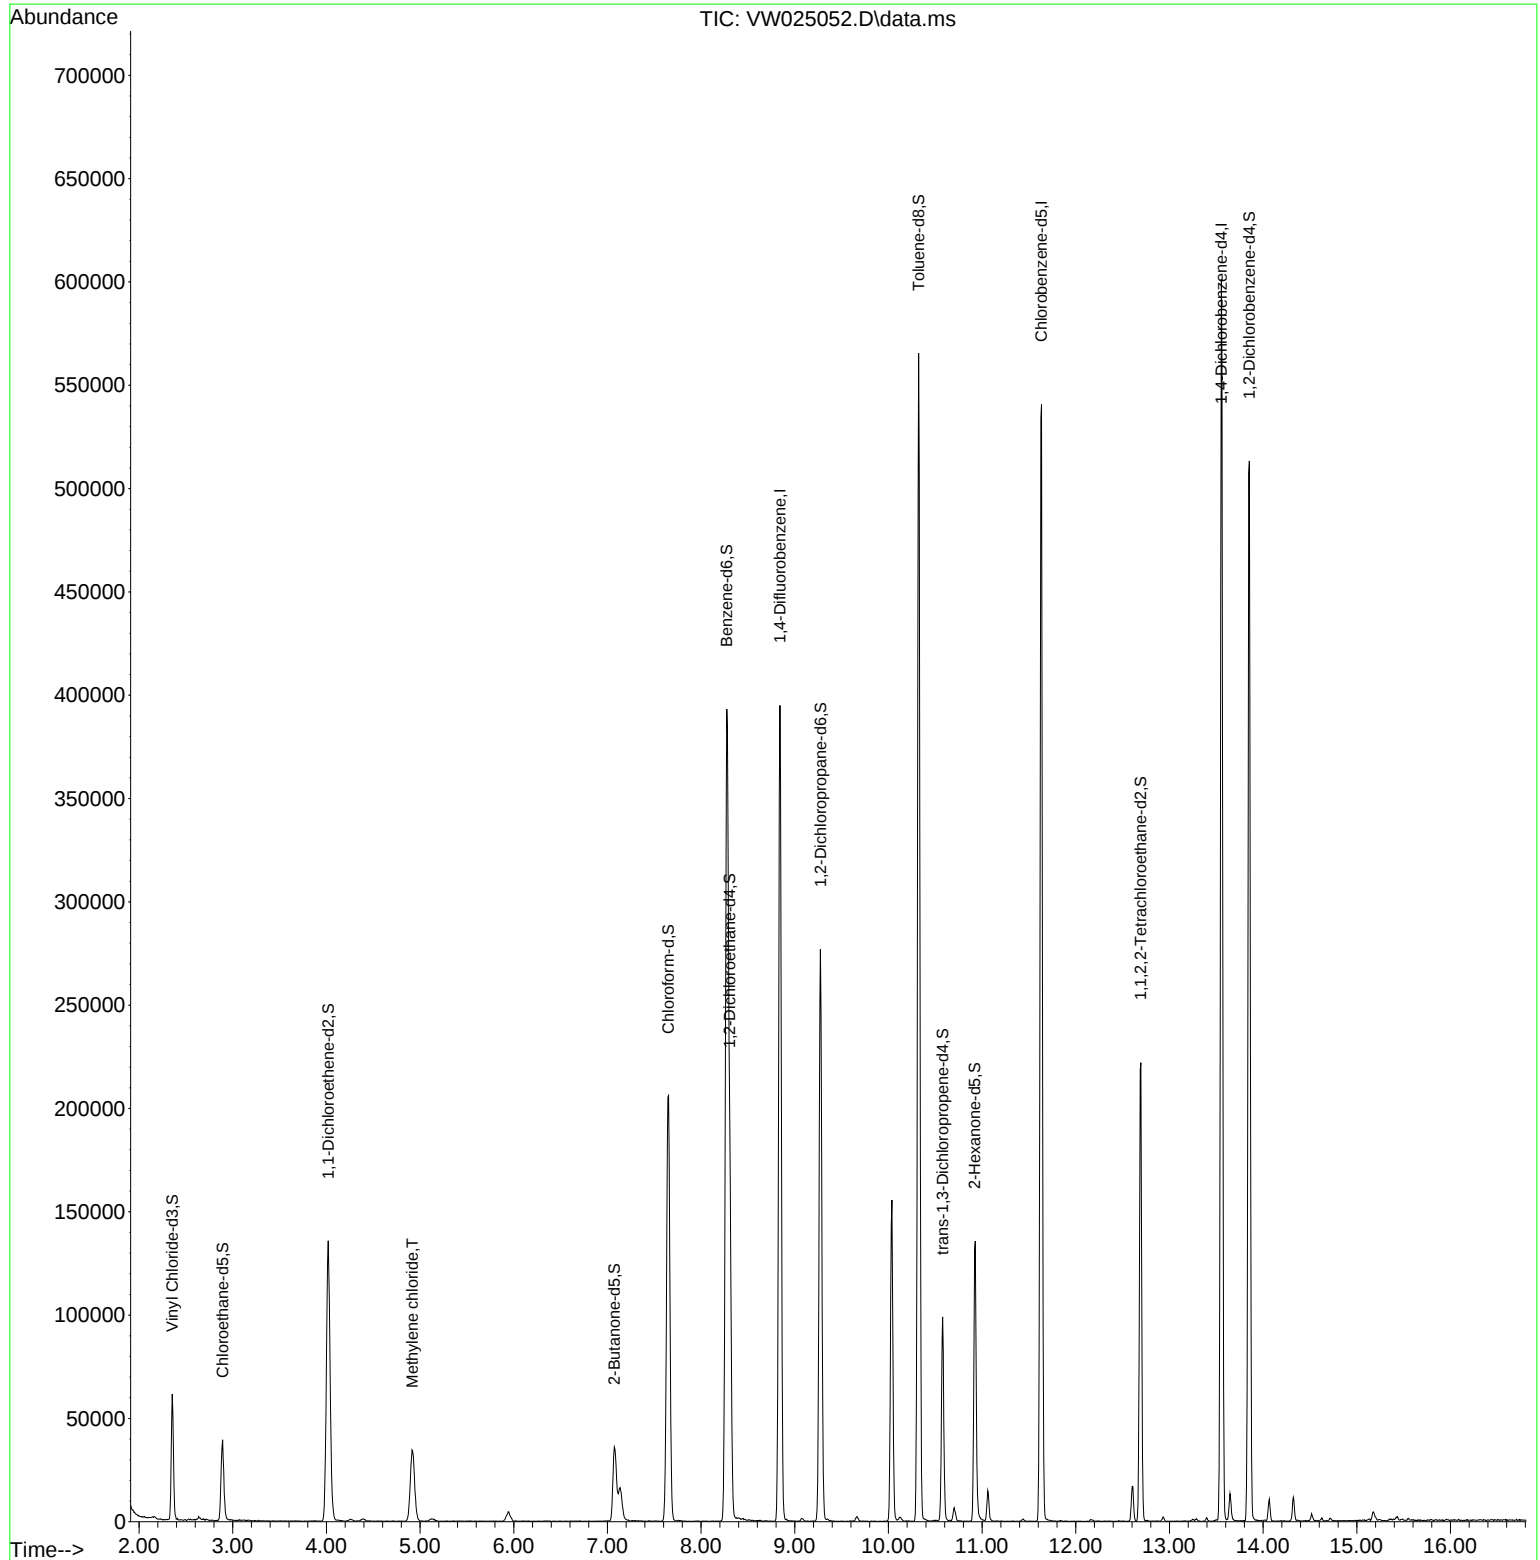

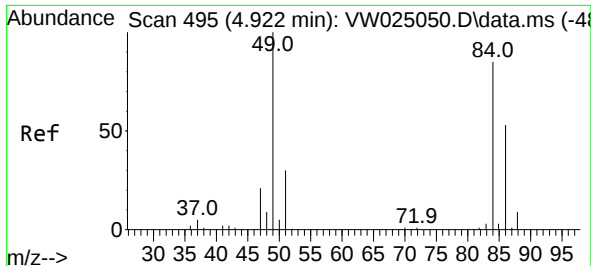

#16
Methylene chloride
Concen: 4.831 ug/L
RT: 4.915 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW025052.D
Acq: 15 Nov 2022 11:05

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Tgt Ion: 84 Resp: 28027
Ion Ratio Lower Upper
84 100
86 62.4 42.6 79.0
49 117.6 81.9 152.1

