

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
 Data File : VW031021.D
 Acq On : 15 Nov 2024 13:03
 Operator : SY/MD
 Sample : VW1115SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 16 00:36:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 16 00:35:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	408561	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	387169	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	174084	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	75430	11.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	45.040%
7) Chloroethane-d5	2.704	69	45	0.009	ug/L	-0.20
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.040%#
11) 1,1-Dichloroethene-d2	4.015	65	40006	14.469	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.880%
21) 2-Butanone-d5	7.075	46	44091	39.984	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.960%
24) Chloroform-d	7.648	84	213512	17.727	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	70.920%
26) 1,2-Dichloroethane-d4	8.307	65	106385	17.765	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.040%
32) Benzene-d6	8.276	84	414004	17.212	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	68.840%
36) 1,2-Dichloropropane-d6	9.270	67	126431	17.831	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	71.320%
41) Toluene-d8	10.319	98	357744	16.582	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	66.320%
43) trans-1,3-Dichloroprop...	10.575	79	46330	16.120	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	64.480%
47) 2-Hexanone-d5	10.922	63	35899	39.065	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.140%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	96199	19.473	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.880%
66) 1,2-Dichlorobenzene-d4	13.848	152	124138	19.576	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.320%
Target Compounds						Qvalue
37) 1,2-Dichloropropane	9.276	63	14005	2.246	ug/L	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031021.D
Acq On : 15 Nov 2024 13:03
Operator : SY/MD
Sample : VW1115SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 16 00:36:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 16 00:35:12 2024
Response via : Initial Calibration

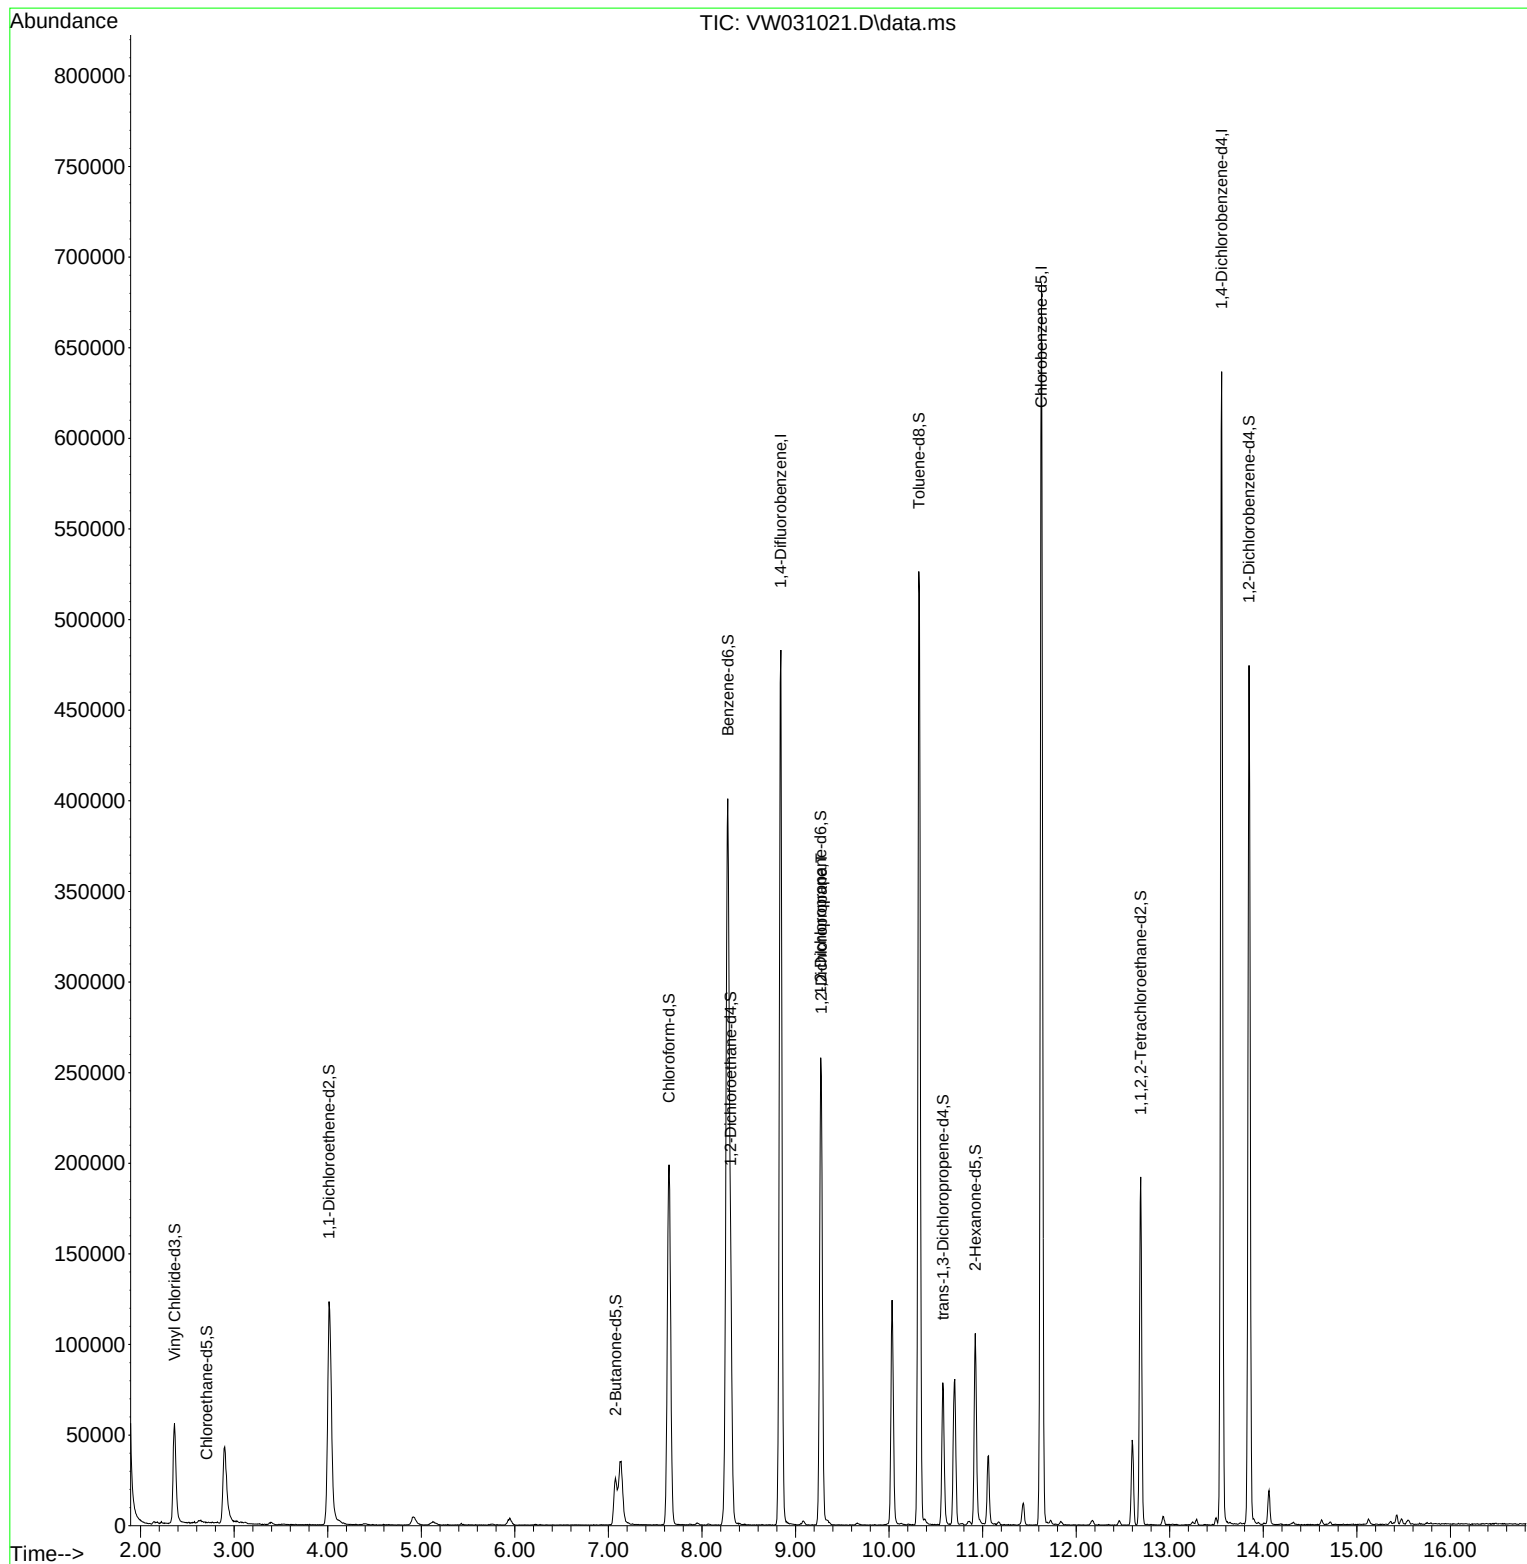

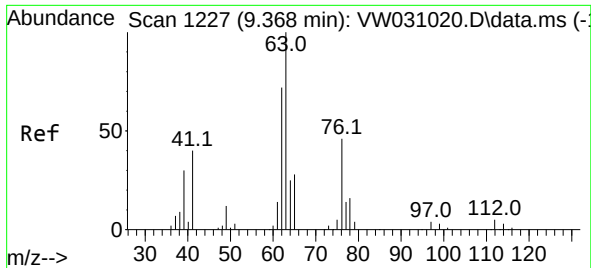

#37

1,2-Dichloropropane

Concen: 2.246 ug/L

RT: 9.276 min Scan# 11

Delta R.T. -0.091 min


Lab File: VW031021.D

Acq: 15 Nov 2024 13:03

Instrument :

MSVOA_W

ClientSampleId :

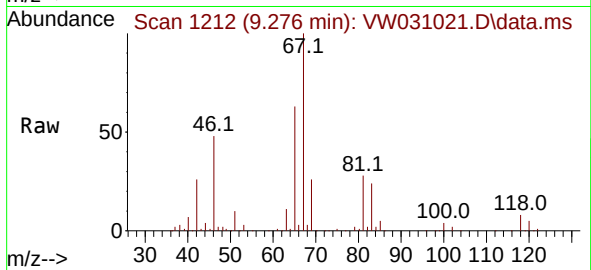

Tgt Ion: 63 Resp: 14005

Ion Ratio Lower Upper

63 100

112 0.8 3.5 5.3#

