

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
 Data File : VW031022.D
 Acq On : 15 Nov 2024 13:36
 Operator : SY/MD
 Sample : P4751-12
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 16 00:36:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 16 00:35:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	409758	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	382873	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	165376	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	74875	11.141	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	44.560%		
7) Chloroethane-d5	2.893	69	65697	12.746	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	51.000%		
11) 1,1-Dichloroethene-d2	4.015	65	39432	14.220	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.880%		
21) 2-Butanone-d5	7.081	46	43521	39.352	ug/L	0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	78.700%		
24) Chloroform-d	7.648	84	211434	17.503	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	70.000%		
26) 1,2-Dichloroethane-d4	8.301	65	108944	18.139	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	72.560%		
32) Benzene-d6	8.270	84	410289	17.249	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	69.000%		
36) 1,2-Dichloropropane-d6	9.270	67	126005	17.970	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	71.880%		
41) Toluene-d8	10.319	98	362870	17.008	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	68.040%		
43) trans-1,3-Dichloroprop...	10.575	79	47507	16.715	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	66.840%		
47) 2-Hexanone-d5	10.922	63	36624	40.302	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	80.600%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	98124	20.086	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.360%		
66) 1,2-Dichlorobenzene-d4	13.849	152	127179	21.112	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.440%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3359	0.364	ug/L	# 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031022.D
Acq On : 15 Nov 2024 13:36
Operator : SY/MD
Sample : P4751-12
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 16 00:36:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 16 00:35:12 2024
Response via : Initial Calibration

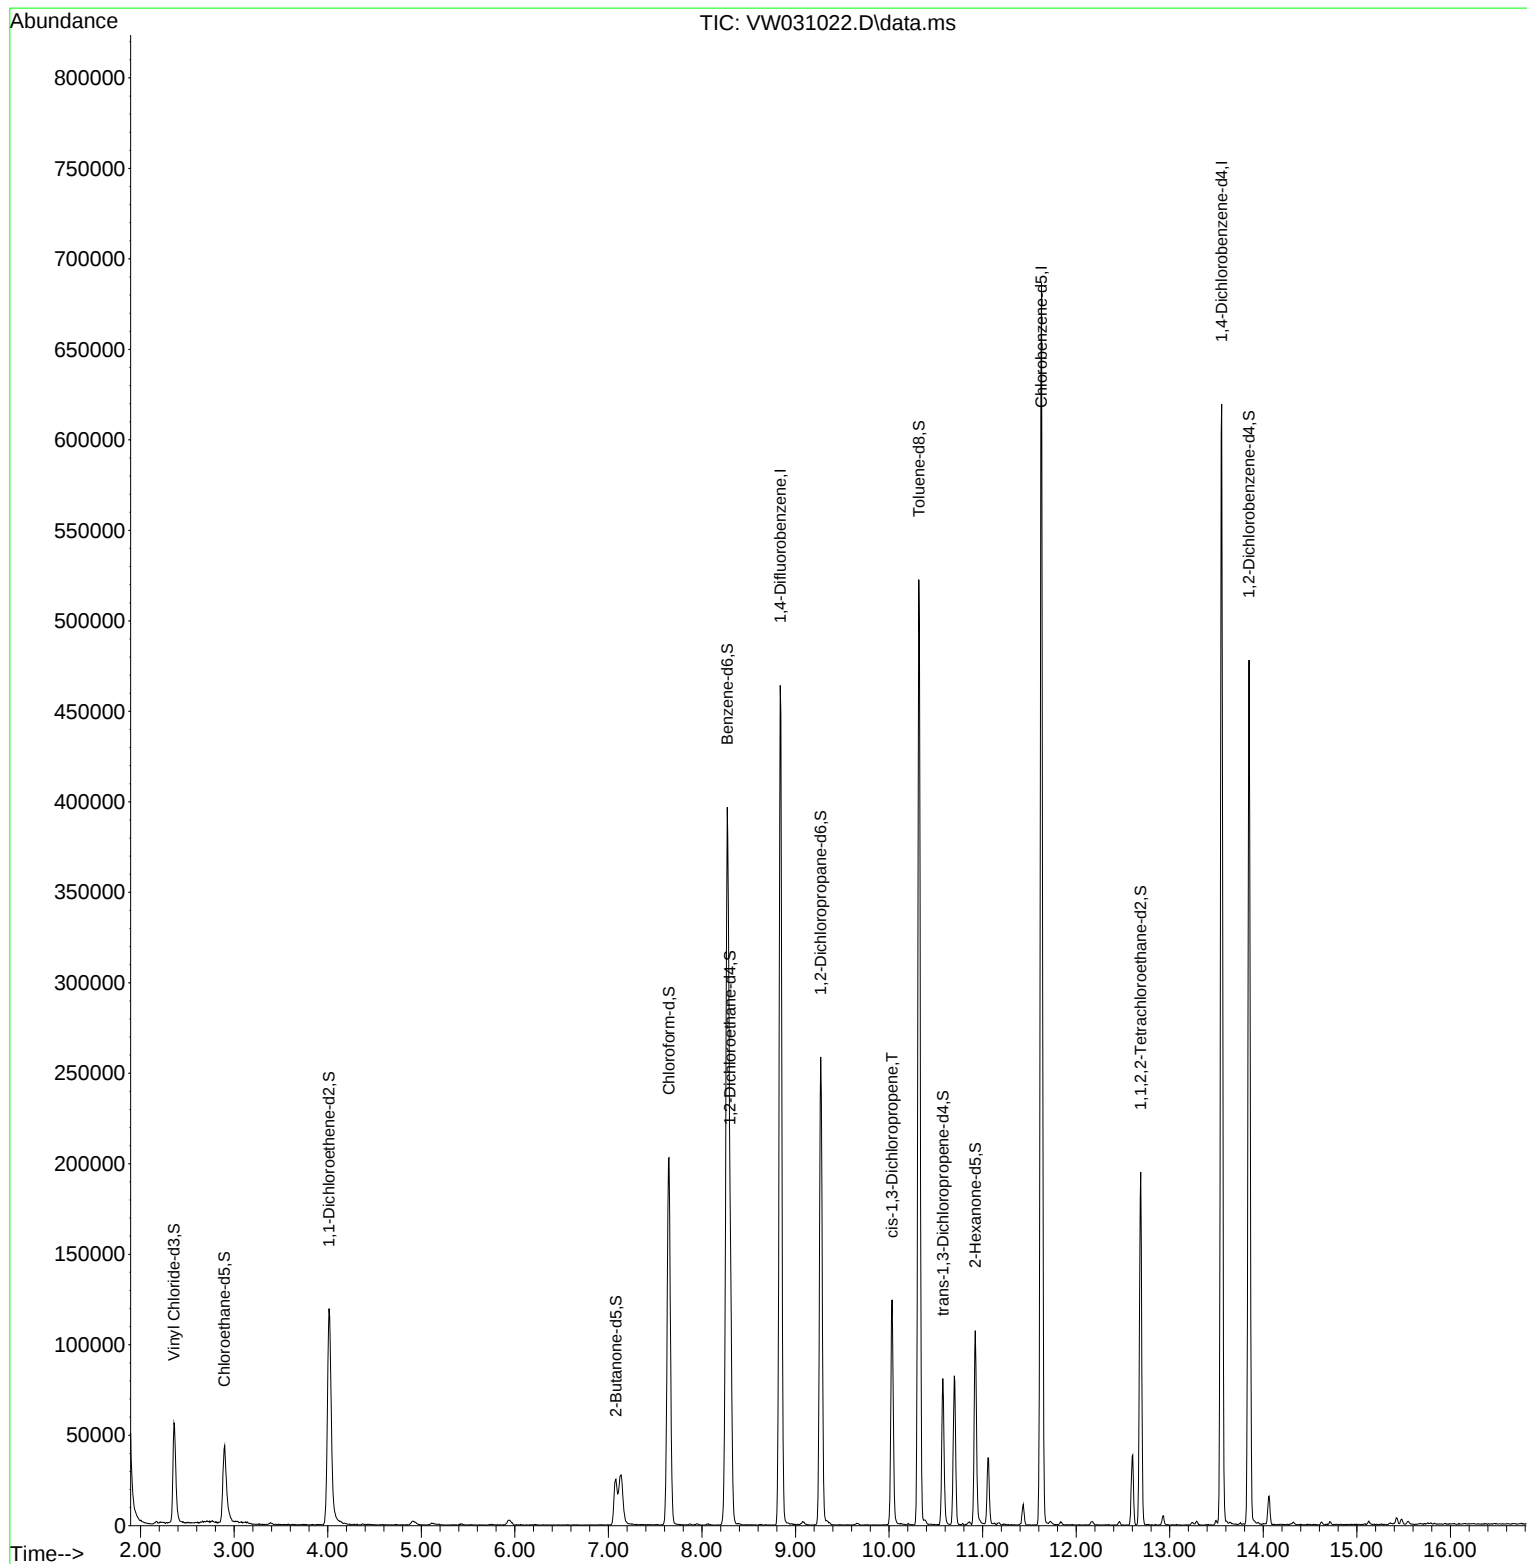

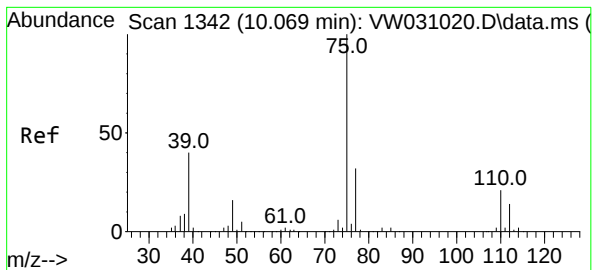

#39
 cis-1,3-Dichloropropene
 Concen: 0.364 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW031022.D
 Acq: 15 Nov 2024 13:36

Instrument :
 MSVOA_W
 ClientSampleId :

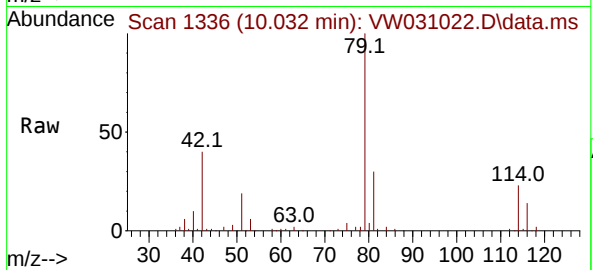

Tgt Ion: 75 Resp: 3359
 Ion Ratio Lower Upper
 75 100
 77 40.7 21.3 39.6#

