

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
 Data File : VW031023.D
 Acq On : 15 Nov 2024 14:00
 Operator : SY/MD
 Sample : P4724-14
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 16 00:36:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 16 00:35:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	404848	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	377115	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	169919	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	86488	13.026	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.120%
7) Chloroethane-d5	2.899	69	75125	14.752	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.000%
11) 1,1-Dichloroethene-d2	4.021	65	45788	16.712	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.840%
21) 2-Butanone-d5	7.075	46	55303	50.612	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.220%
24) Chloroform-d	7.648	84	255127	21.376	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.520%
26) 1,2-Dichloroethane-d4	8.301	65	127469	21.481	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.920%
32) Benzene-d6	8.270	84	480219	20.497	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.000%
36) 1,2-Dichloropropane-d6	9.270	67	150625	21.809	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.240%
41) Toluene-d8	10.319	98	428899	20.410	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.640%
43) trans-1,3-Dichloroprop...	10.575	79	57593	20.573	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.280%
47) 2-Hexanone-d5	10.922	63	45839	51.212	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.420%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	121197	25.188	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	154606	24.979	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.920%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	4164	0.458	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031023.D
Acq On : 15 Nov 2024 14:00
Operator : SY/MD
Sample : P4724-14
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 16 00:36:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 16 00:35:12 2024
Response via : Initial Calibration

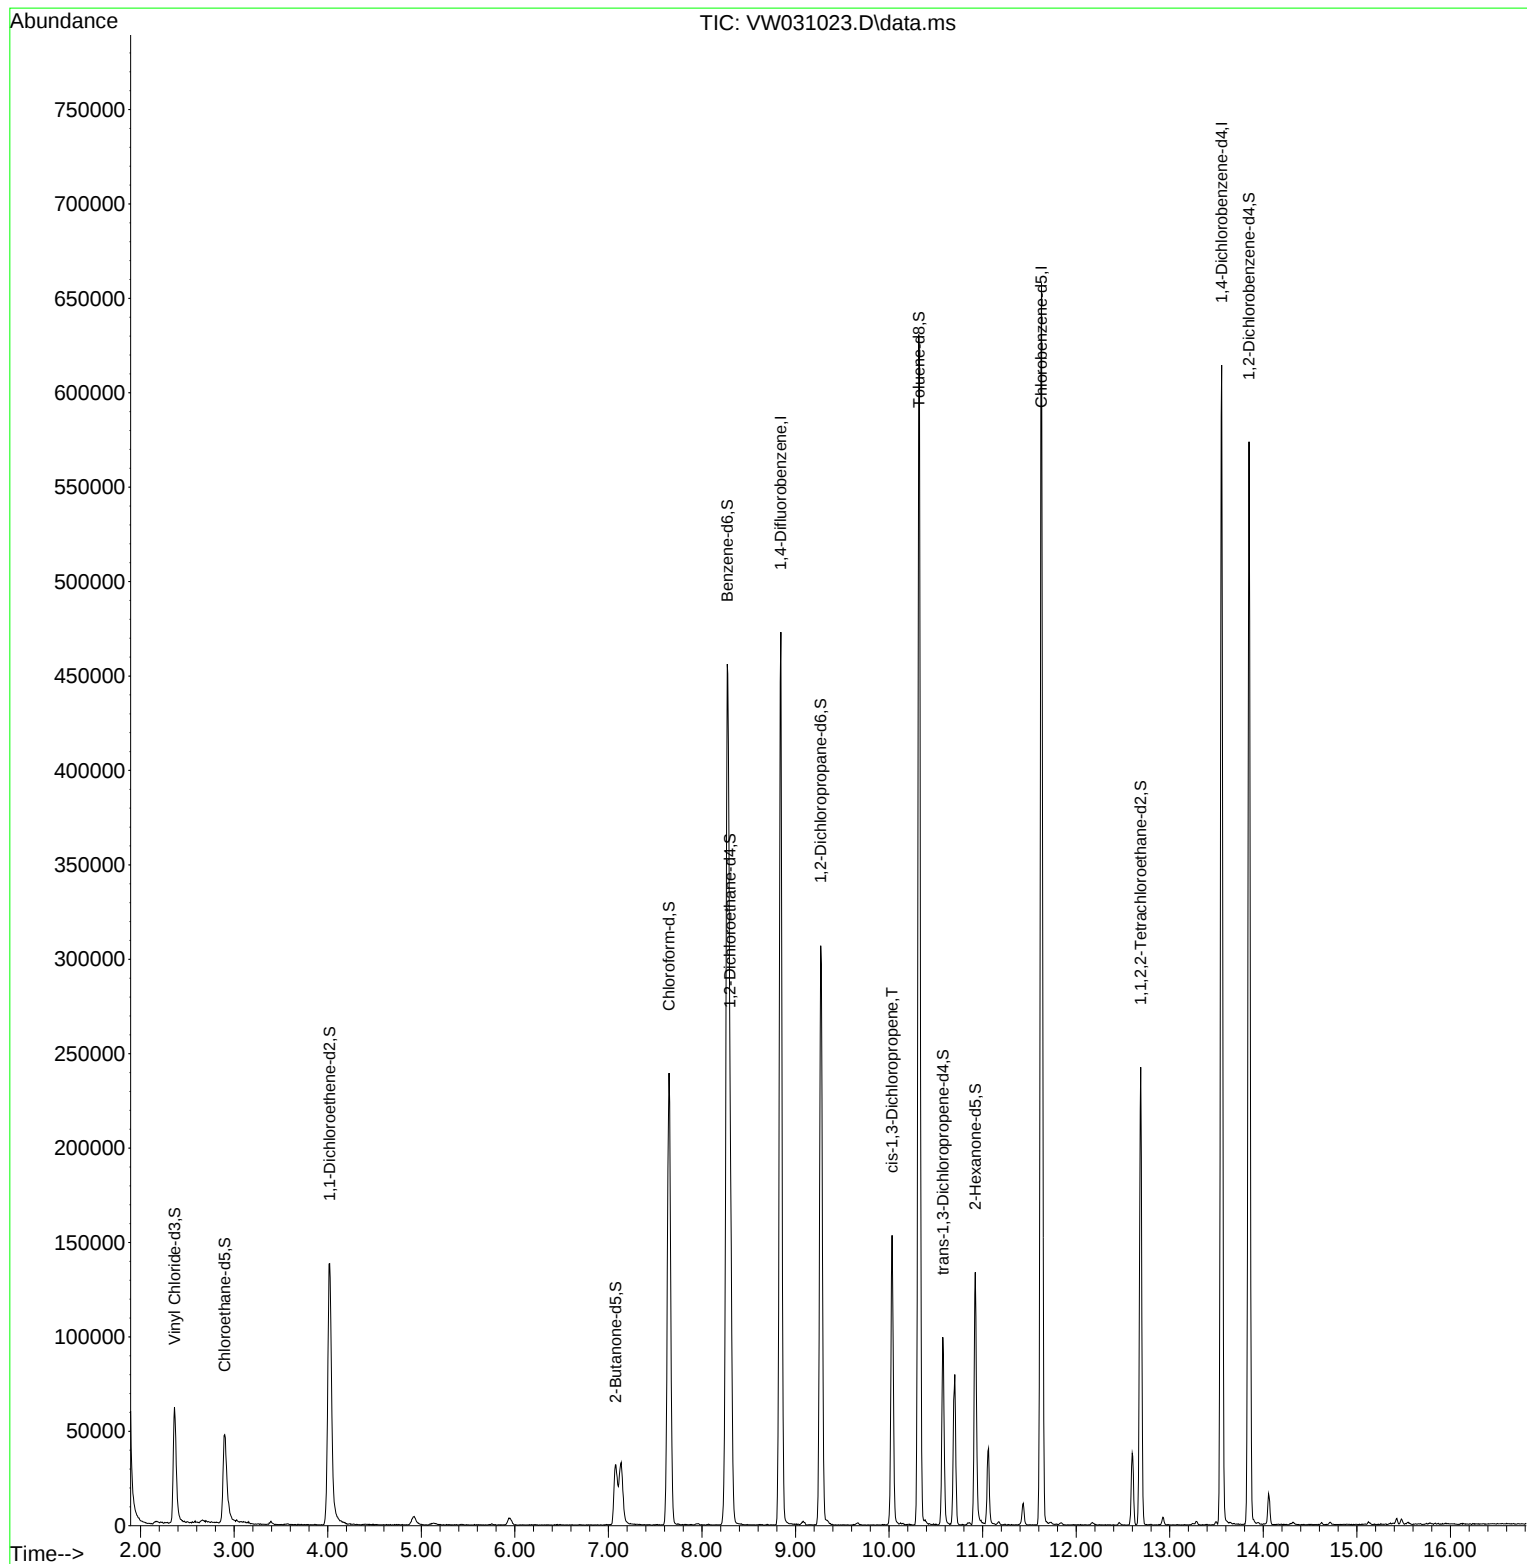

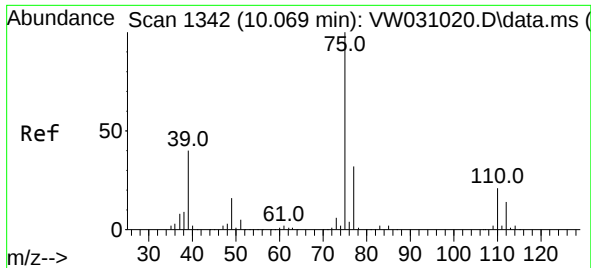

#39

cis-1,3-Dichloropropene

Concen: 0.458 ug/L

RT: 10.032 min Scan# 11

Delta R.T. -0.037 min


Lab File: VW031023.D

Acq: 15 Nov 2024 14:00

Instrument :

MSVOA_W

ClientSampleId :

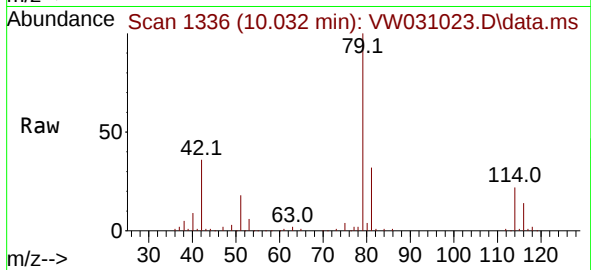

Tgt Ion: 75 Resp: 4164

Ion Ratio Lower Upper

75 100

77 38.1 21.3 39.6

