




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031021.D
Acq On : 15 Nov 2024 13:03
Operator : SY/MD
Sample : VW1115SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK597

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:36:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 16 00:35:12 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/17/2024
Supervised By :Mahesh Dadoda 11/19/2024

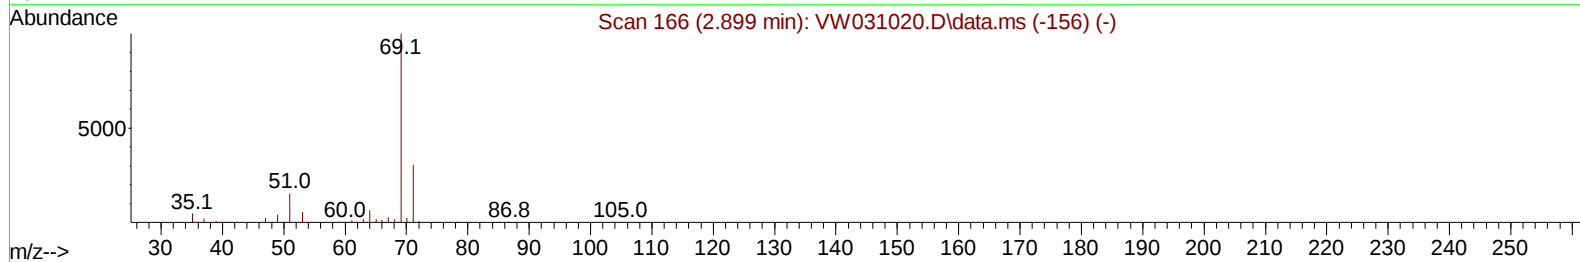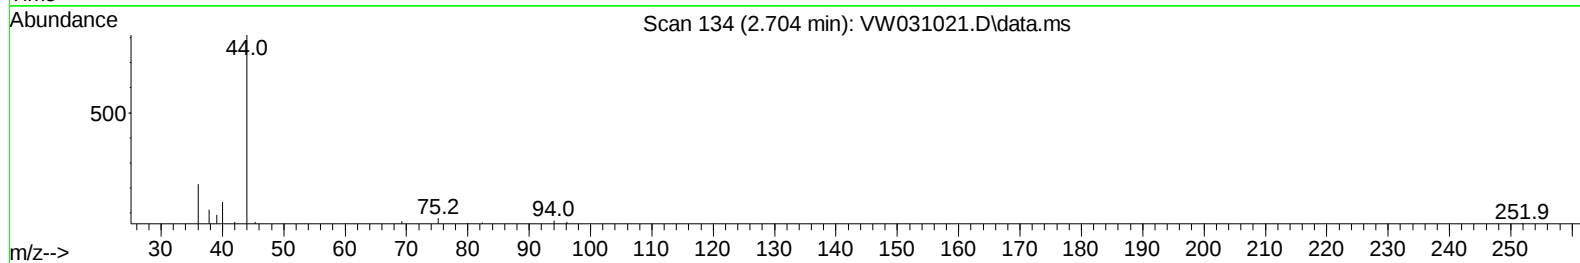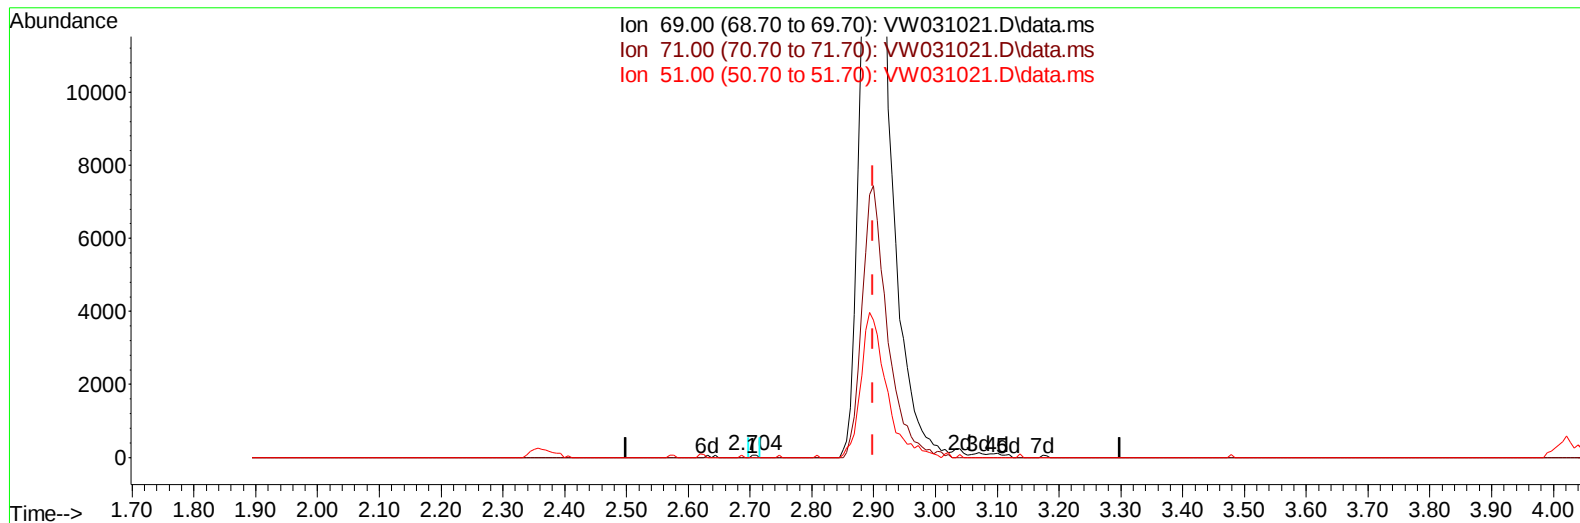

TIC: VW031021.D\data.ms

(7) Chloroethane-d5 (S)

2.704min (-0.195) 0.01 ug/L

response 45

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.80	46808.89#
51.00	24.10	25275.56#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031021.D
Acq On : 15 Nov 2024 13:03
Operator : SY/MD
Sample : VW1115SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK597

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:36:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 16 00:35:12 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 11/17/2024
Supervised By :Mahesh Dadoda 11/19/2024

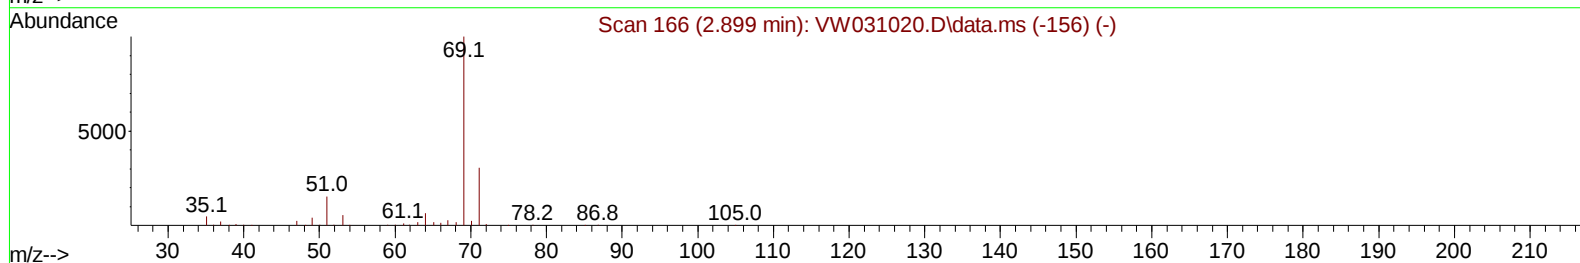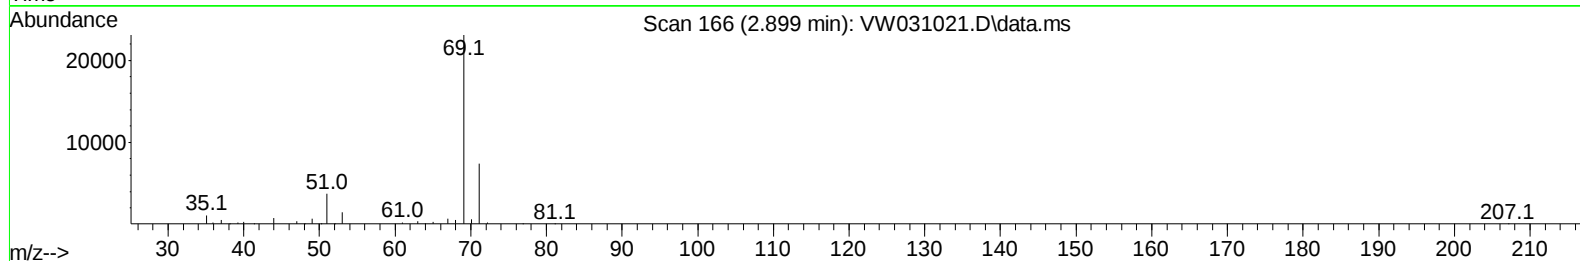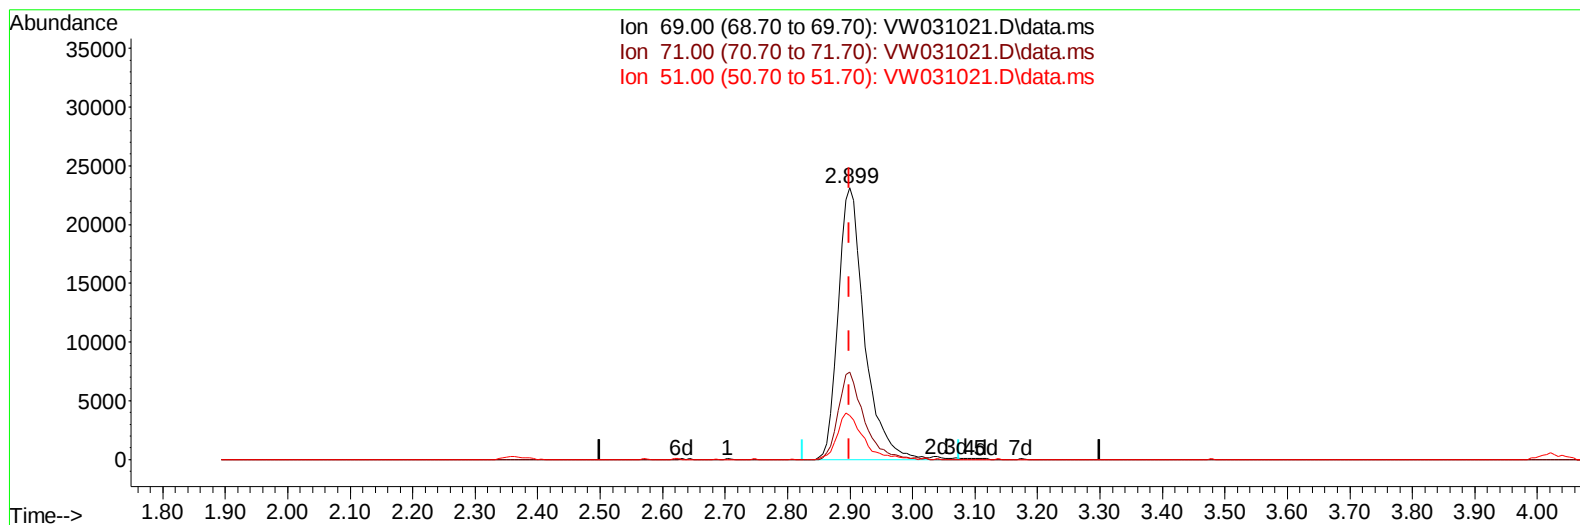

TIC: VW031021.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (+ 0.000) 13.16 ug/L m

response 67654

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.80	31.13
51.00	24.10	16.81#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw111524\
 Data File : VW031021.D
 Acq On : 15 Nov 2024 13:03
 Operator : SY/MD
 Sample : VW1115SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK597

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 11/17/2024
 Supervised By :Mahesh Dadoda 11/19/2024

Quant Time: Nov 16 00:36:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 16 00:35:12 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		408561	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		387169	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		174084	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		75430	11.257	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	45.040%		
7) Chloroethane-d5	2.899	69		67654m	13.164	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	52.640%		
11) 1,1-Dichloroethene-d2	4.015	65		40006	14.469	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.880%		
21) 2-Butanone-d5	7.075	46		44091	39.984	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	79.960%		
24) Chloroform-d	7.648	84		213512	17.727	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	70.920%		
26) 1,2-Dichloroethane-d4	8.307	65		106385	17.765	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	71.040%		
32) Benzene-d6	8.276	84		414004	17.212	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	68.840%		
36) 1,2-Dichloropropane-d6	9.270	67		126431	17.831	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	71.320%		
41) Toluene-d8	10.319	98		357744	16.582	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	66.320%		
43) trans-1,3-Dichloroprop...	10.575	79		46330	16.120	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	64.480%		
47) 2-Hexanone-d5	10.922	63		35899	39.065	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	78.140%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		96199	19.473	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	77.880%		
66) 1,2-Dichlorobenzene-d4	13.848	152		124138	19.576	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	78.320%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031021.D
Acq On : 15 Nov 2024 13:03
Operator : SY/MD
Sample : VW1115SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK597

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 11/17/2024
Supervised By :Mahesh Dadoda 11/19/2024

Quant Time: Nov 16 00:36:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 16 00:35:12 2024
Response via : Initial Calibration

