

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
 Data File : VW031033.D
 Acq On : 15 Nov 2024 18:34
 Operator : SY/MD
 Sample : P4872-11
 Misc : 3.86g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E29X9

Quant Time: Nov 16 00:40:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 16 00:35:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	518070	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	425313	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	144648	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	95345	11.221	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	44.880%
7) Chloroethane-d5	2.899	69	77254	11.855	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	47.400%
11) 1,1-Dichloroethene-d2	4.015	65	46939	13.388	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.560%
21) 2-Butanone-d5	7.075	46	76601	54.783	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.560%
24) Chloroform-d	7.648	84	247012	16.173	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	64.680%
26) 1,2-Dichloroethane-d4	8.307	65	135214	17.806	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.240%
32) Benzene-d6	8.276	84	465026	17.600	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.400%
36) 1,2-Dichloropropane-d6	9.270	67	148583	19.076	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.320%
41) Toluene-d8	10.318	98	381633	16.103	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	64.400%
43) trans-1,3-Dichloroprop...	10.574	79	53265	16.870	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.480%
47) 2-Hexanone-d5	10.922	63	59187	58.631	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.260%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	126610	23.331	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	94587	17.952	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	71.800%#
Target Compounds					Qvalue	
13) Acetone	4.112	43	41208	24.130	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031033.D
Acq On : 15 Nov 2024 18:34
Operator : SY/MD
Sample : P4872-11
Misc : 3.86g/10mL/MSVOA_W/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29X9

Quant Time: Nov 16 00:40:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 16 00:35:12 2024
Response via : Initial Calibration

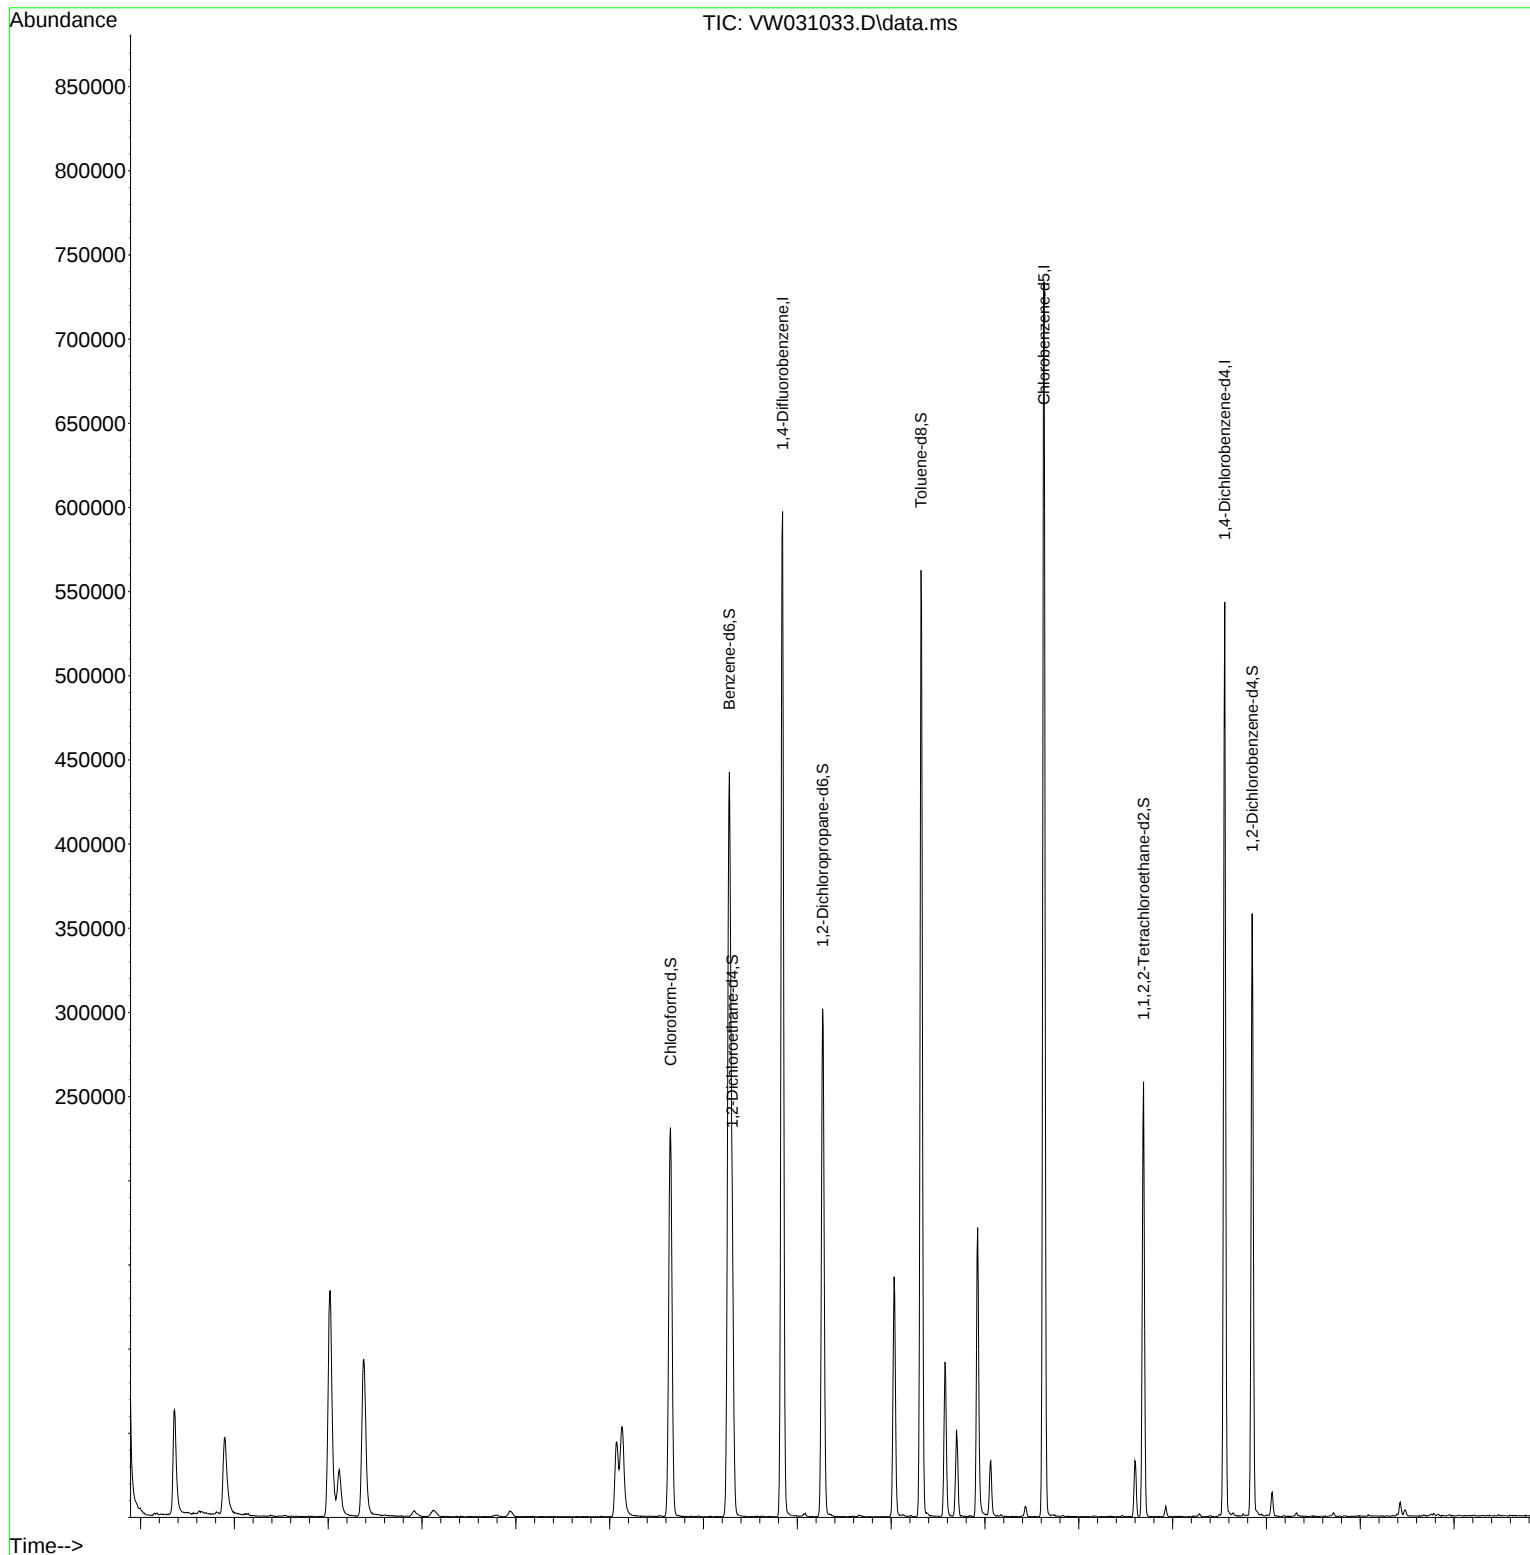

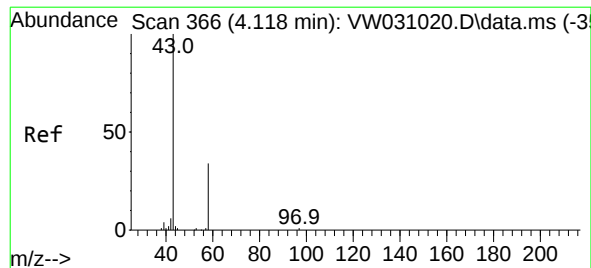

#13
 Acetone
 Concen: 24.130 ug/L
 RT: 4.112 min Scan# 36
 Delta R.T. -0.006 min
 Lab File: VW031033.D
 Acq: 15 Nov 2024 18:34

Instrument :
 MSVOA_W
 ClientSampleId :
 E29X9

Tgt Ion: 43 Resp: 41208
 Ion Ratio Lower Upper
 43 100
 58 35.0 0.0 62.6

