

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
 Data File : VW031034.D
 Acq On : 15 Nov 2024 18:58
 Operator : SY/MD
 Sample : P4872-12
 Misc : 6.67g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y0

Quant Time: Nov 16 00:40:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Nov 16 00:35:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	336214	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	214097	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	47623	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	79859	14.482	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	57.920%		
7) Chloroethane-d5	2.899	69	61839	14.622	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	58.480%		
11) 1,1-Dichloroethene-d2	4.021	65	37506	16.484	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	65.920%		
21) 2-Butanone-d5	7.075	46	47000	51.794	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	103.580%		
24) Chloroform-d	7.648	84	177241	17.882	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	71.520%		
26) 1,2-Dichloroethane-d4	8.307	65	88644	17.988	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	71.960%		
32) Benzene-d6	8.270	84	323301	24.307	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.240%		
36) 1,2-Dichloropropane-d6	9.270	67	101950	26.001	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	104.000%		
41) Toluene-d8	10.319	98	236844	19.852	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	79.400%		
43) trans-1,3-Dichloroprop...	10.575	79	31093	19.563	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	78.240%		
47) 2-Hexanone-d5	10.922	63	33023	64.986	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	129.980%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	86238	31.569	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	126.280%#		
66) 1,2-Dichlorobenzene-d4	13.849	152	46685	26.912	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	107.640%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	10675	9.632	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031034.D
Acq On : 15 Nov 2024 18:58
Operator : SY/MD
Sample : P4872-12
Misc : 6.67g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E29Y0

Quant Time: Nov 16 00:40:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Nov 16 00:35:12 2024
Response via : Initial Calibration

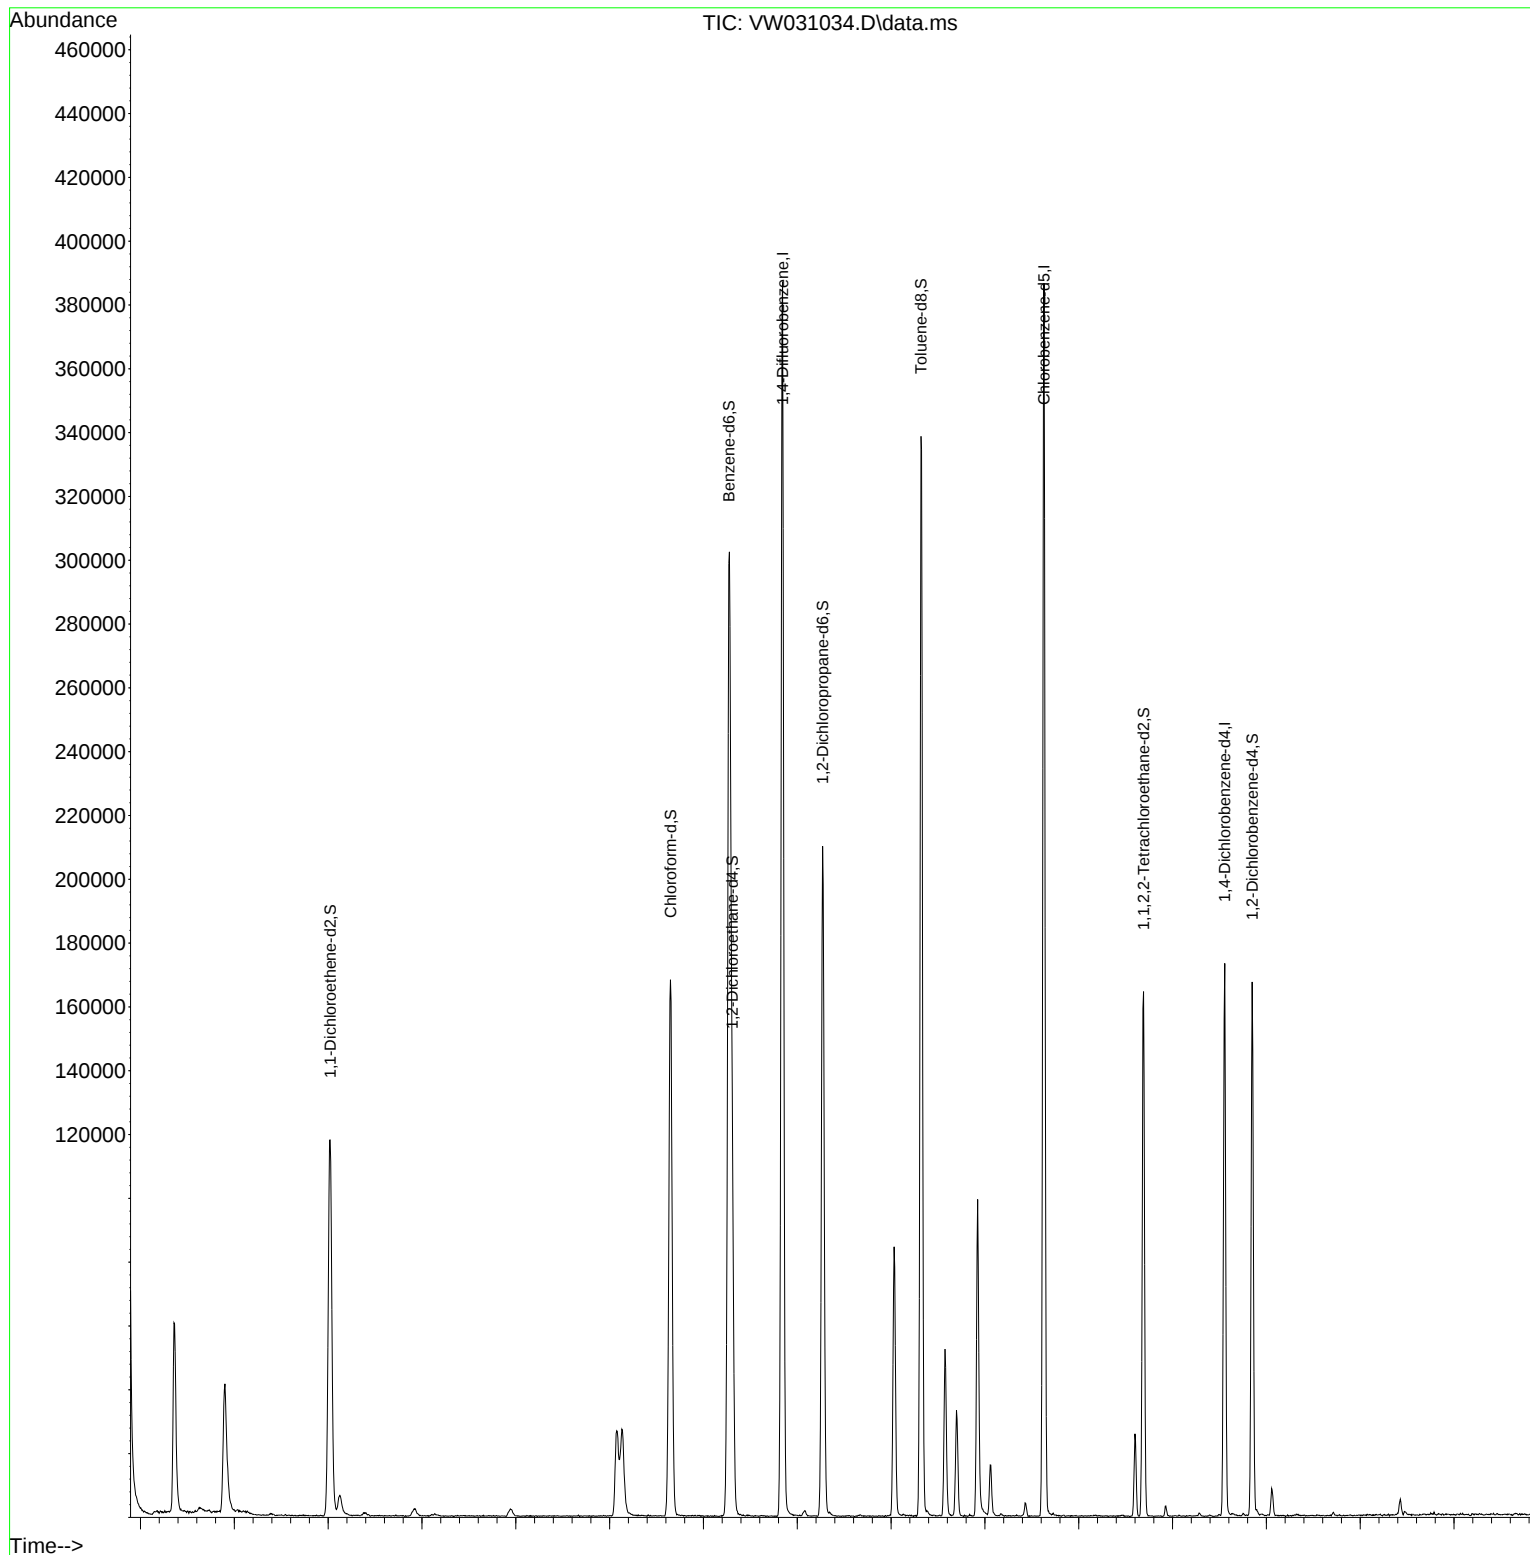

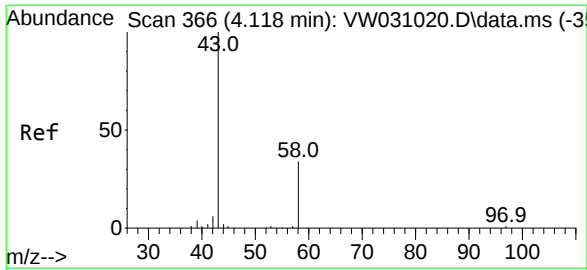

#13
 Acetone
 Concen: 9.632 ug/L
 RT: 4.125 min Scan# 36
 Delta R.T. 0.006 min
 Lab File: VW031034.D
 Acq: 15 Nov 2024 18:58

Instrument :
 MSVOA_W
 ClientSampleId :
 E29Y0

Tgt Ion: 43 Resp: 10675
 Ion Ratio Lower Upper
 43 100
 58 30.9 0.0 62.6

