
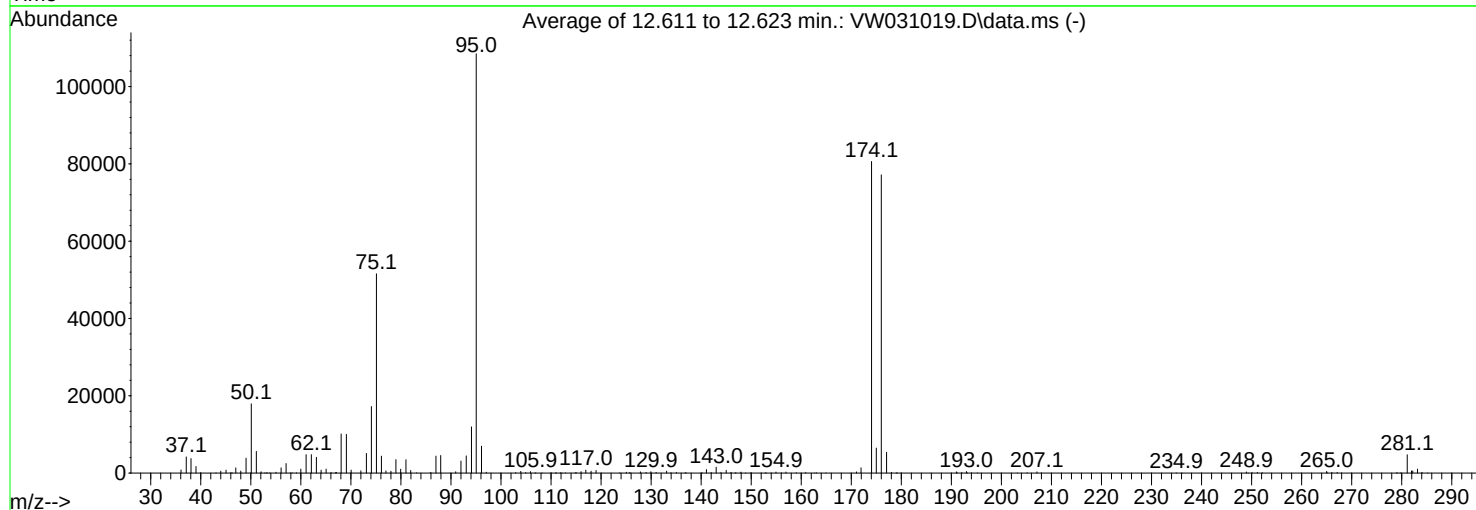


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111524\
Data File : VW031019.D
Acq On : 15 Nov 2024 09:35
Operator : SY/MD
Sample : BFB599
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB599

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM110424SMA.M
Title : SFAM01.0
Last Update : Tue Nov 19 00:28:30 2024

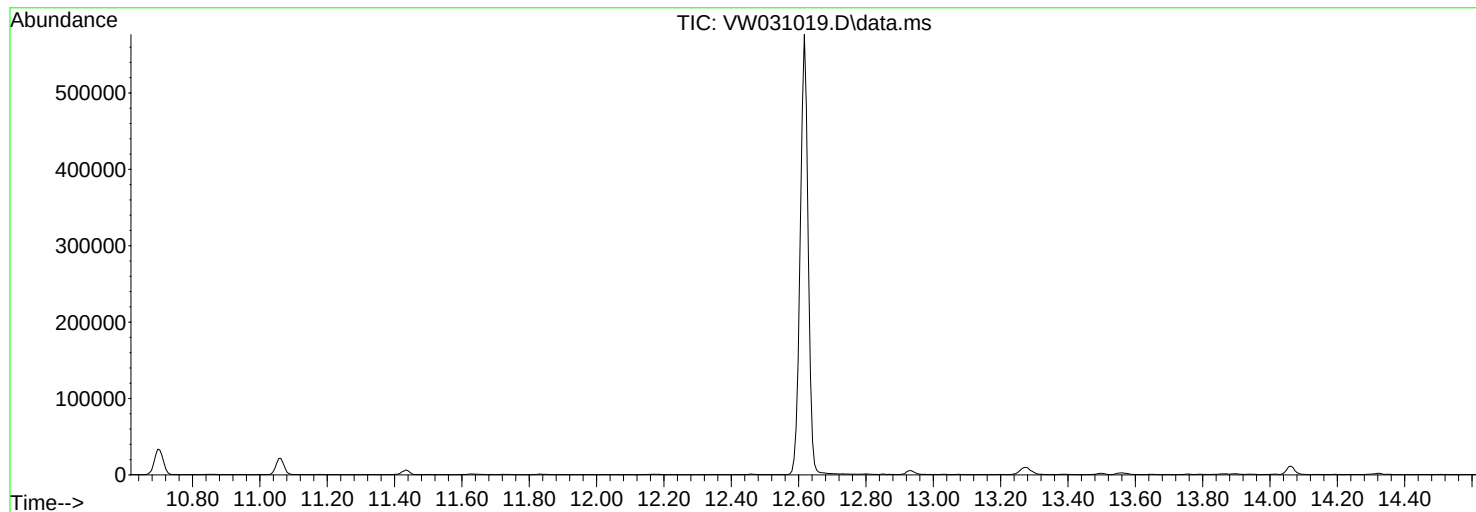

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	17922	PASS
75	95	30	80	47.5	51560	PASS
95	95	100	100	100.0	108493	PASS
96	95	5	9	6.4	6952	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.3	80611	PASS
175	174	5	9	8.0	6476	PASS
176	174	95	101	95.7	77152	PASS
177	176	5	9	7.0	5402	PASS

m/z	Abundance
40.00	210.0
43.90	177.0

Instrument :
MSVOA_W
ClientSampleId :
BFB599

m/z	Abundance
36.10	833.0
37.10	4121.0
38.10	3689.0
39.10	1995.0
40.00	354.0
43.00	100.0
44.00	732.0
45.00	901.0
46.10	204.0
47.00	1473.0
48.00	536.0
49.10	3709.0
50.10	18184.0
51.10	5537.0
52.10	282.0
53.10	89.0
53.80	72.0
55.10	154.0
56.00	1261.0
57.00	2357.0
58.30	87.0
59.10	184.0
60.00	1163.0
61.10	4937.0
62.10	4629.0
63.10	3960.0
64.00	764.0
65.00	1074.0
66.10	113.0
66.90	368.0
68.10	10056.0
69.10	9770.0
70.00	766.0
72.00	518.0
73.10	5310.0
74.10	17056.0
75.10	48744.0
76.10	4290.0
77.00	630.0
78.20	334.0
79.00	3903.0
80.00	1014.0
81.00	3425.0
81.90	655.0
83.10	108.0
85.90	132.0
87.00	4022.0
88.00	4651.0
91.00	338.0
92.00	3118.0
93.10	4416.0
94.10	10904.0
95.00	101144.0
96.10	6912.0
97.10	250.0
103.00	183.0
104.00	538.0
105.10	197.0
105.90	433.0
106.80	63.0
108.20	77.0
110.00	90.0
110.90	82.0
111.90	87.0
112.90	59.0
114.90	225.0
116.00	320.0
117.00	888.0
118.00	477.0
118.90	712.0
125.00	411.0
125.60	206.0
127.90	299.0
129.10	132.0
129.90	288.0
131.00	162.0
133.10	810.0
135.00	183.0
136.80	164.0
140.20	60.0
141.00	932.0
142.00	110.0
143.00	1403.0
143.90	145.0
145.00	779.0
146.00	144.0
146.80	170.0
147.90	231.0
150.00	124.0
152.80	93.0
154.00	53.0
155.00	251.0

Instrument :
MSVOA_W
ClientSampleId :
BFB599

156.10	59.0
157.00	160.0
159.10	57.0
160.90	110.0
162.70	94.0
163.10	104.0
164.90	102.0
171.10	331.0
171.90	1284.0
174.10	67568.0
175.00	5581.0
176.00	60784.0
177.00	4902.0
178.20	135.0
179.00	223.0
191.00	650.0
192.10	136.0
193.00	767.0
194.10	124.0
195.20	106.0
203.20	52.0
205.20	127.0
207.10	541.0
208.00	96.0
234.90	64.0
236.10	54.0
248.90	429.0
250.10	173.0
251.20	270.0
252.20	81.0
265.00	807.0
266.00	305.0
267.20	303.0
268.00	82.0
278.90	151.0
279.70	137.0
281.10	7391.0
282.20	1639.0
283.20	1692.0
284.00	241.0
285.20	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB599

m/z	Abundance
36.00	813.0
37.10	4676.0
38.00	4432.0
39.00	1789.0
40.10	231.0
43.10	62.0
44.10	714.0
45.00	819.0
46.00	185.0
47.00	1590.0
48.10	540.0
49.10	4407.0
50.10	19872.0
51.10	6551.0
52.00	507.0
52.80	125.0
53.30	88.0
55.10	284.0
56.10	1604.0
57.00	3060.0
58.20	142.0
59.10	75.0
60.00	1103.0
61.10	5281.0
62.10	5529.0
63.10	4478.0
64.10	1046.0
65.00	1087.0
66.00	122.0
67.10	313.0
68.00	11140.0
69.10	10809.0
70.10	963.0
72.00	582.0
73.10	5455.0
74.10	19440.0
75.10	59632.0
76.10	5341.0
77.00	583.0
78.00	617.0
79.00	3832.0
80.00	1103.0
81.00	3906.0
82.00	774.0
83.20	88.0
86.00	194.0
87.00	4968.0
87.90	5062.0
90.90	418.0
92.00	3453.0
93.00	5055.0
94.10	14015.0
95.10	126304.0
96.10	7976.0
97.00	164.0
102.90	149.0
103.90	411.0
104.90	138.0
105.90	395.0
107.00	70.0
110.00	69.0
110.90	89.0
111.80	139.0
112.90	85.0
114.80	132.0
115.10	128.0
116.00	435.0
116.90	779.0
118.00	567.0
119.00	805.0
123.80	86.0
125.10	151.0
125.70	138.0
127.80	370.0
128.90	196.0
130.00	499.0
131.00	162.0
133.10	506.0
133.90	134.0
135.00	135.0
137.00	147.0
140.10	147.0
141.00	873.0
142.10	150.0
143.00	1809.0
144.00	95.0
145.00	742.0
146.00	164.0
147.00	135.0
148.00	268.0
148.90	54.0
150.00	128.0

Instrument :
MSVOA_W
ClientSampleId :
BFB599

152.00	57.0
152.80	66.0
154.90	309.0
157.00	301.0
159.00	106.0
160.80	173.0
163.00	103.0
165.00	60.0
171.10	419.0
172.00	1677.0
174.00	90816.0
175.00	7350.0
176.00	84144.0
177.10	5624.0
178.00	238.0
179.20	69.0
180.00	63.0
191.00	329.0
192.10	132.0
193.00	477.0
194.00	73.0
205.10	99.0
207.10	290.0
208.00	70.0
235.00	72.0
249.00	349.0
250.10	137.0
251.10	196.0
252.20	86.0
265.00	594.0
266.10	179.0
267.00	184.0
279.20	69.0
281.10	4390.0
281.90	991.0
283.10	1014.0
284.10	200.0

Instrument :
MSVOA_W
ClientSampleId :
BFB599

m/z	Abundance
36.00	767.0
37.10	3713.0
38.10	3164.0
39.00	1352.0
40.10	256.0
44.00	560.0
45.10	605.0
46.30	78.0
47.00	1009.0
47.90	472.0
49.00	3455.0
50.10	15710.0
51.10	4715.0
52.00	272.0
53.20	180.0
55.00	243.0
56.10	1233.0
57.10	1993.0
57.90	95.0
60.00	821.0
61.00	4089.0
62.10	4155.0
63.10	3815.0
64.00	516.0
65.10	917.0
66.00	96.0
67.10	256.0
68.00	9173.0
69.10	9498.0
70.10	615.0
72.00	678.0
73.10	4477.0
74.10	15170.0
75.10	46304.0
76.10	3520.0
77.00	510.0
77.90	489.0
79.00	2712.0
79.90	910.0
81.00	3028.0
81.90	586.0
86.00	161.0
87.00	4205.0
88.00	3941.0
91.00	310.0
92.00	2779.0
93.00	3886.0
94.10	10972.0
95.10	98032.0
96.10	5969.0
97.00	272.0
102.90	67.0
104.00	398.0
104.80	130.0
105.90	290.0
106.90	70.0
111.10	110.0
111.80	55.0
112.20	64.0
115.00	168.0
116.00	349.0
117.00	704.0
118.00	455.0
119.10	553.0
123.70	56.0
124.90	77.0
125.90	60.0
127.90	319.0
129.00	213.0
130.00	296.0
131.00	166.0
133.00	216.0
134.00	78.0
135.10	159.0
136.80	151.0
140.10	99.0
141.10	909.0
141.90	115.0
143.00	1385.0
144.00	62.0
145.00	661.0
145.90	251.0
146.90	50.0
147.90	274.0
148.90	69.0
149.90	108.0
153.00	101.0
154.90	255.0
156.00	52.0
156.90	350.0
158.90	116.0
161.00	149.0

Instrument :
MSVOA_W
ClientSampleId :
BFB599

170.90	201.0
172.00	1143.0
174.00	83448.0
175.00	6498.0
176.00	86528.0
177.00	5680.0
178.00	104.0
191.20	171.0
192.00	56.0
193.20	175.0
207.10	107.0
248.80	132.0
249.30	113.0
251.30	85.0
265.20	174.0
266.90	58.0
279.00	57.0
281.10	2454.0
282.00	707.0
283.10	399.0
284.00	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB599