

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111622\
 Data File : VW025064.D
 Acq On : 16 Nov 2022 17:39
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK586

Quant Time: Nov 17 00:41:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 00:39:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	478331	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	429694	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	203902	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	101124	18.835	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.360%
7) Chloroethane-d5	2.885	69	70021	22.263	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.040%
11) 1,1-Dichloroethene-d2	4.019	63	180640	13.507	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.040%
21) 2-Butanone-d5	7.080	46	89252	49.256	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.520%
24) Chloroform-d	7.653	84	309533	21.323	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.280%
26) 1,2-Dichloroethane-d4	8.305	65	163246	20.090	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.360%
32) Benzene-d6	8.274	84	633682	23.008	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	92.040%
36) 1,2-Dichloropropane-d6	9.274	67	198147	24.554	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.200%
41) Toluene-d8	10.323	98	560993	21.879	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.520%
43) trans-1,3-Dichloroprop...	10.579	79	72982	20.395	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.600%
47) 2-Hexanone-d5	10.926	63	69478	49.840	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.680%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	154086	23.913	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.640%
66) 1,2-Dichlorobenzene-d4	13.853	152	179728	22.937	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.760%
Target Compounds						
16) Methylene chloride	4.921	84	34999	4.121	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111622\
Data File : VW025064.D
Acq On : 16 Nov 2022 17:39
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK586

Quant Time: Nov 17 00:41:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 00:39:48 2022
Response via : Initial Calibration

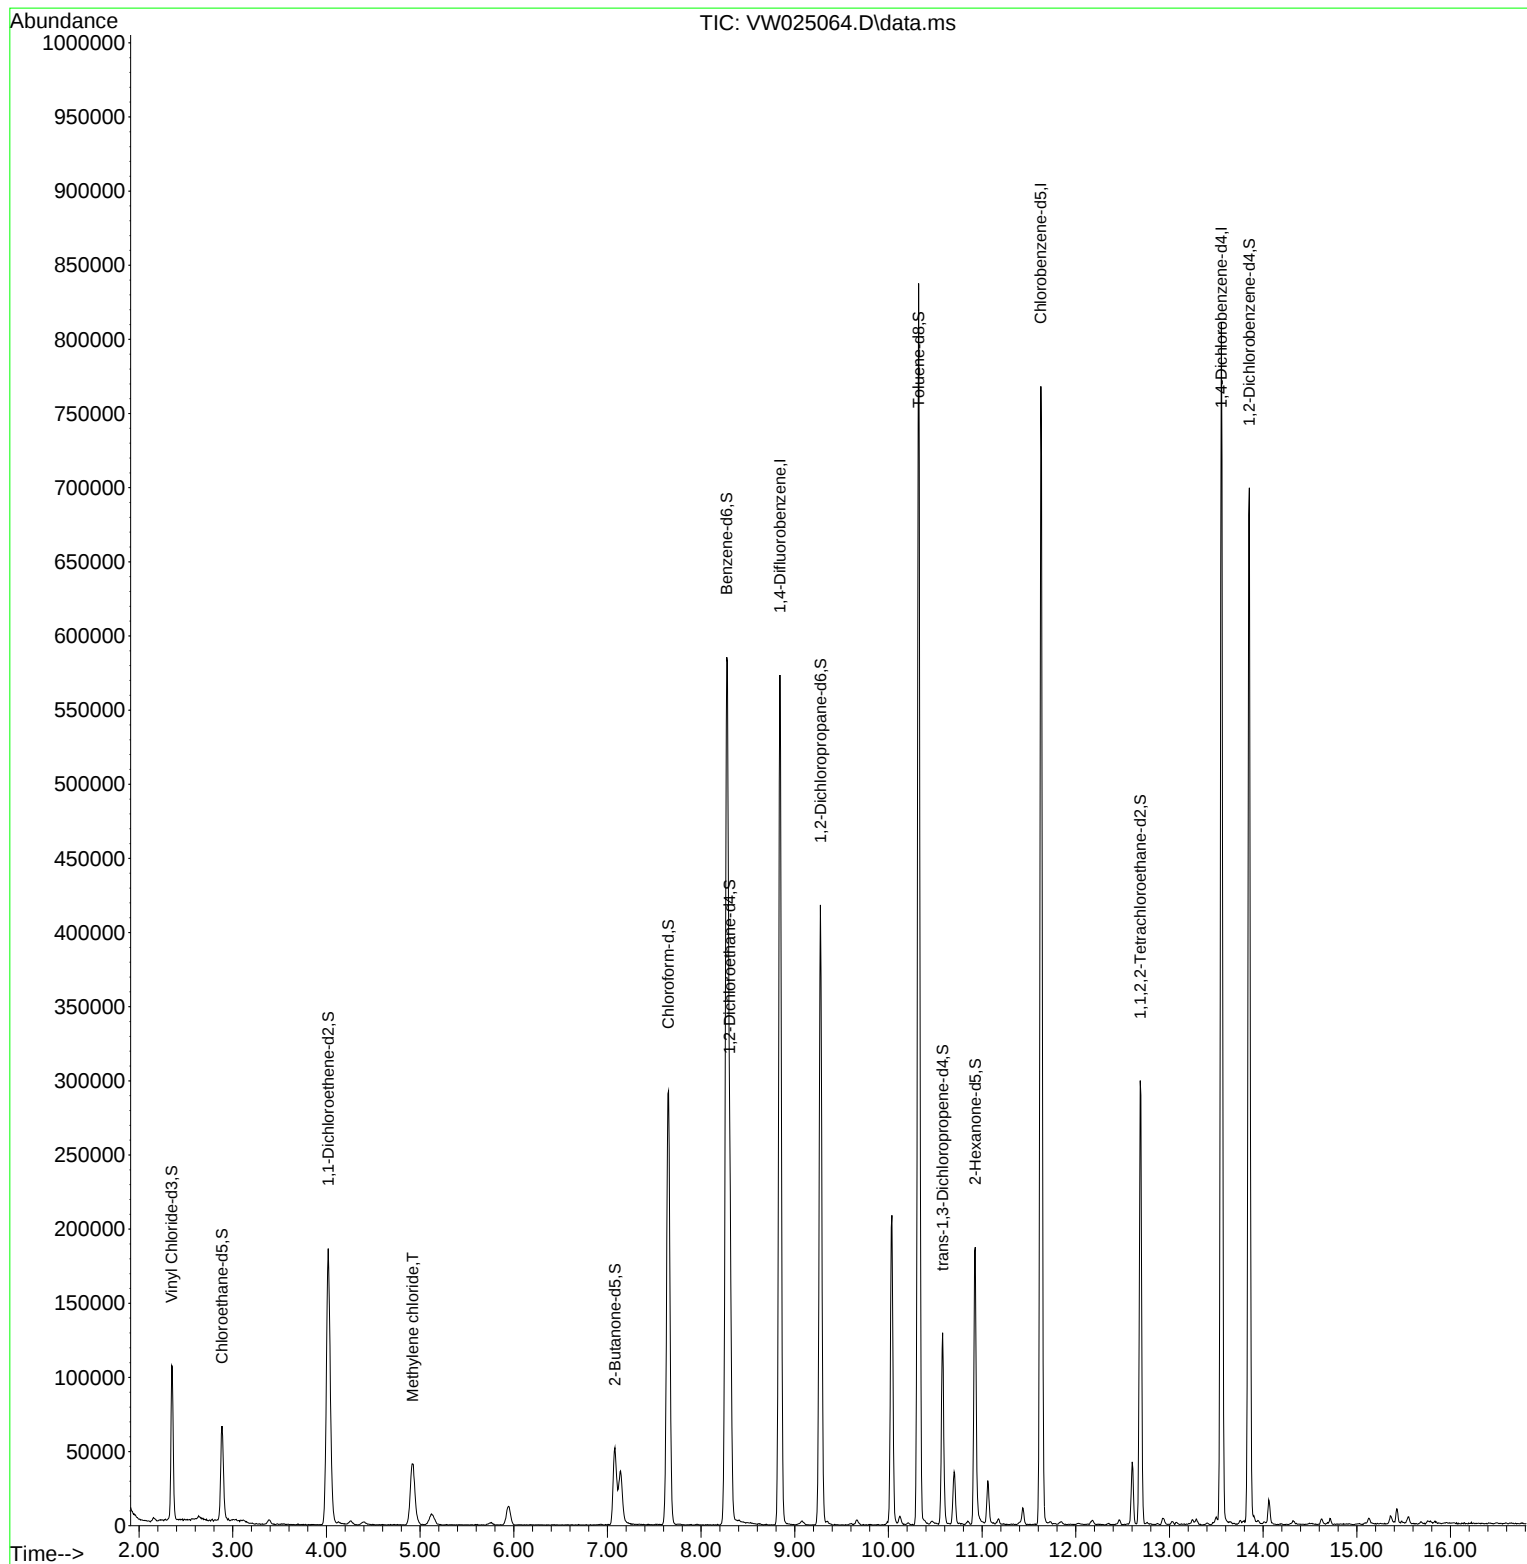

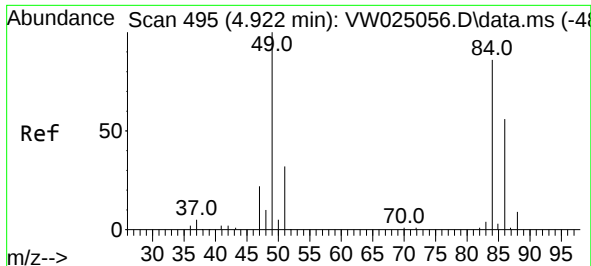

#16
Methylene chloride
Concen: 4.121 ug/L
RT: 4.921 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW025064.D
Acq: 16 Nov 2022 17:39

Instrument :
MSVOA_W
ClientSampleId :
VIBLK586

Tgt Ion: 84 Resp: 34999
Ion Ratio Lower Upper
84 100
86 65.7 42.6 79.0
49 121.1 81.9 152.1

