

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111622\
 Data File : VW025065.D
 Acq On : 16 Nov 2022 18:03
 Operator : SY/VA
 Sample : N5658-06
 Misc : 5.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ESQT6

Quant Time: Nov 17 00:41:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 00:39:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	476988	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	422591	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	194529	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	90909	16.980	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.920%
7) Chloroethane-d5	2.885	69	63866	20.364	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.440%
11) 1,1-Dichloroethene-d2	4.019	63	166685	12.499	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.000%
21) 2-Butanone-d5	7.074	46	91772	50.789	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.580%
24) Chloroform-d	7.647	84	297612	20.559	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.240%
26) 1,2-Dichloroethane-d4	8.305	65	154337	19.047	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.200%
32) Benzene-d6	8.275	84	574153	21.197	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.800%
36) 1,2-Dichloropropane-d6	9.275	67	183852	23.165	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.680%
41) Toluene-d8	10.323	98	513884	20.378	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.520%
43) trans-1,3-Dichloroprop...	10.579	79	69737	19.816	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.280%
47) 2-Hexanone-d5	10.927	63	69024	50.347	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.700%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	156558	24.705	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	159829	21.380	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.520%
Target Compounds						
16) Methylene chloride	4.916	84	31564	3.727	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111622\
Data File : VW025065.D
Acq On : 16 Nov 2022 18:03
Operator : SY/VA
Sample : N5658-06
Misc : 5.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ESQT6

Quant Time: Nov 17 00:41:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 00:39:48 2022
Response via : Initial Calibration

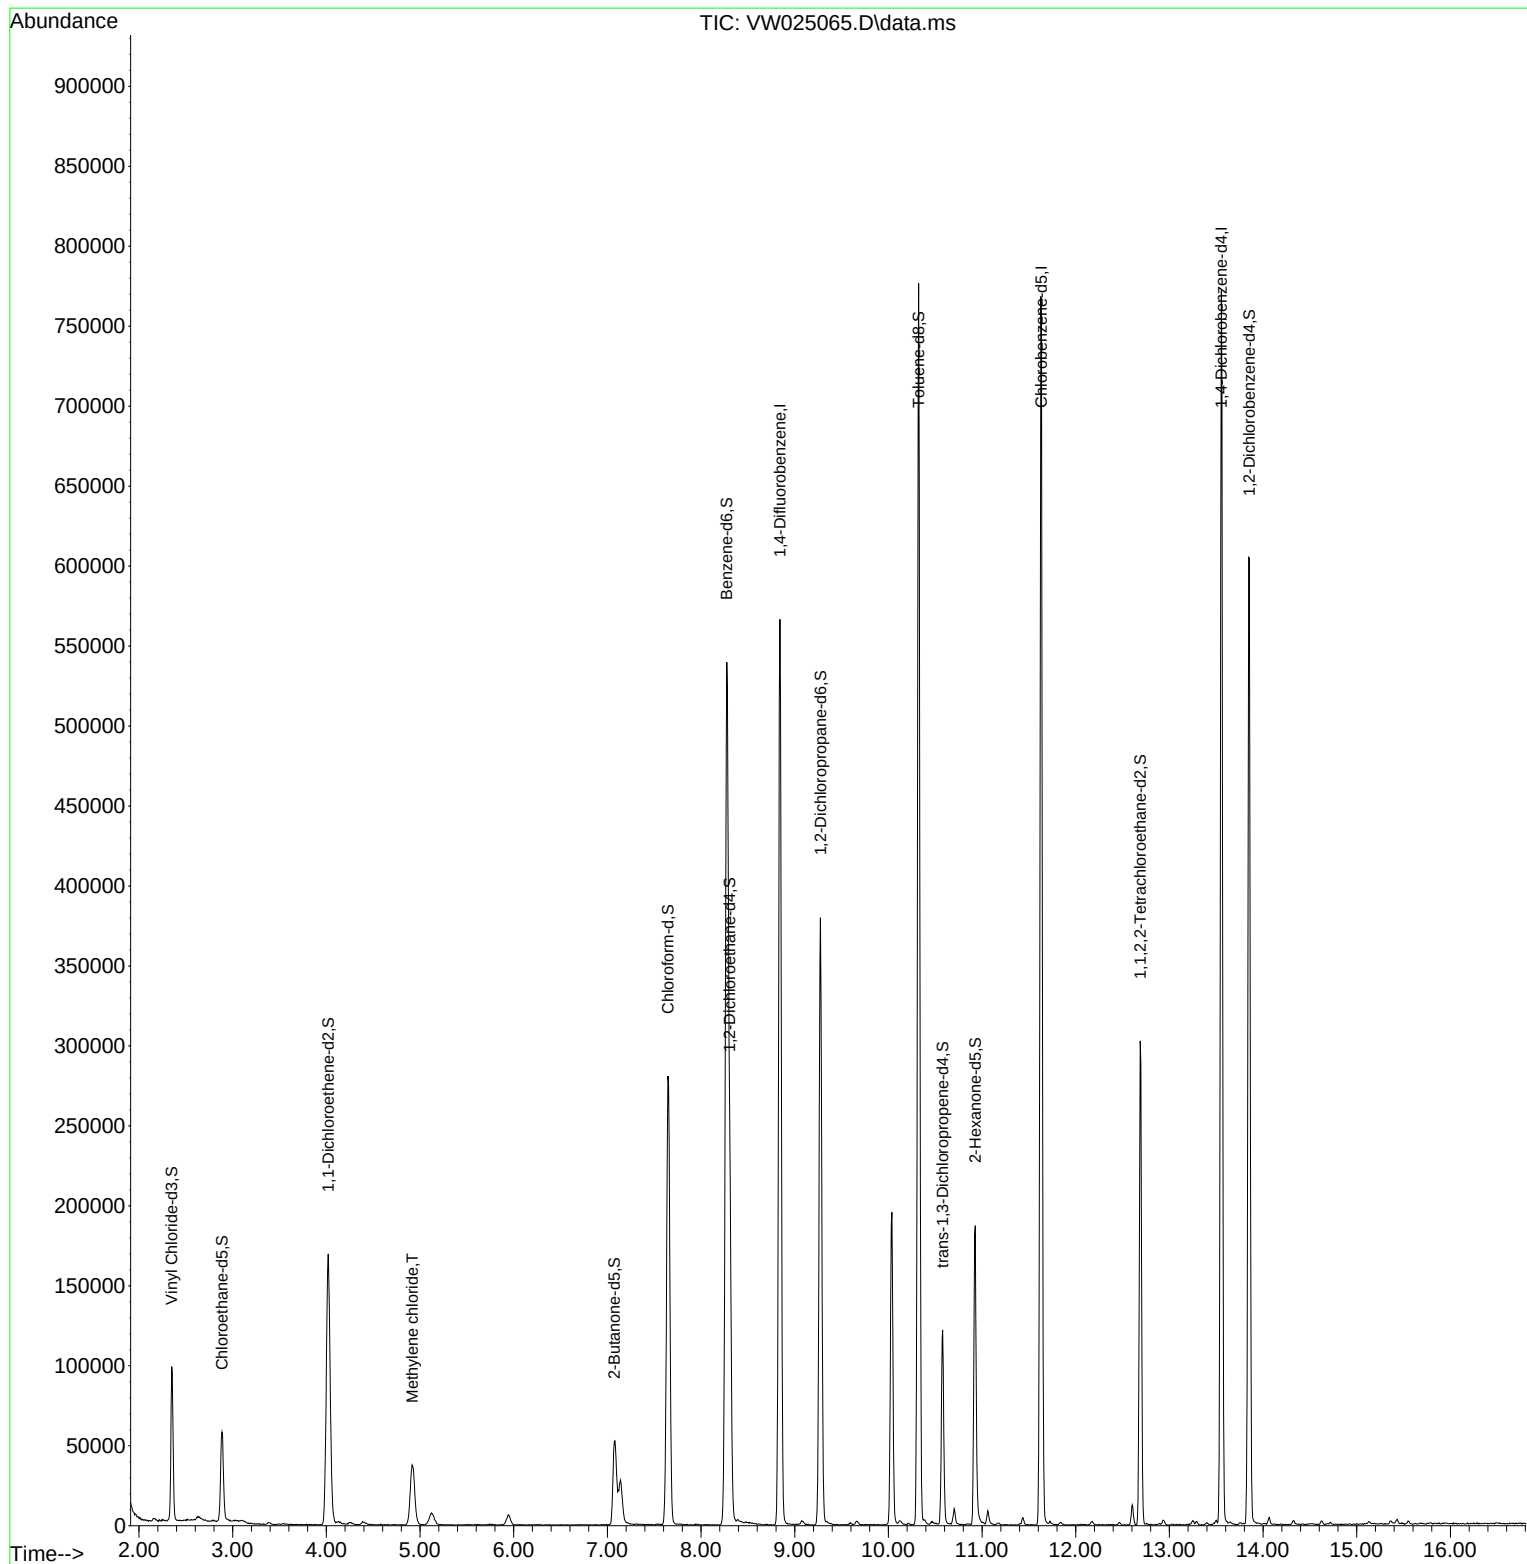

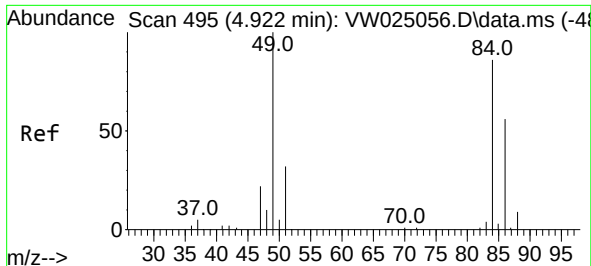

#16
Methylene chloride
Concen: 3.727 ug/L
RT: 4.916 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW025065.D
Acq: 16 Nov 2022 18:03

Instrument :
MSVOA_W
ClientSampleId :
ESQT6

Tgt Ion: 84 Resp: 31564
Ion Ratio Lower Upper
84 100
86 57.9 42.6 79.0
49 121.8 81.9 152.1

