
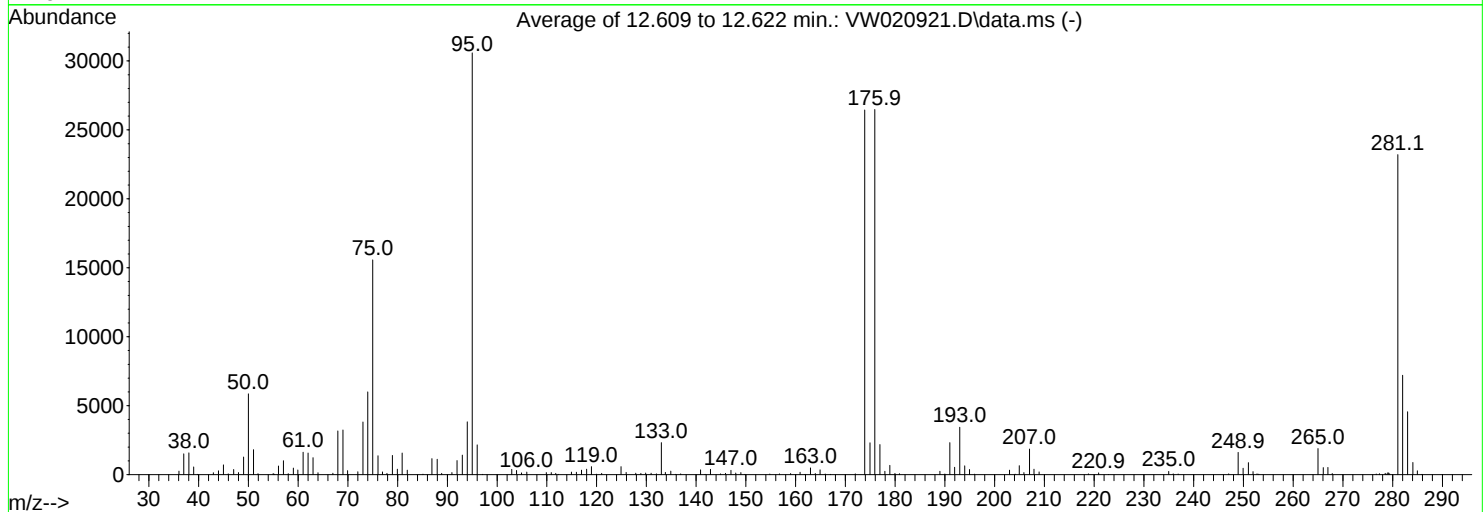


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111821\
Data File : VW020921.D
Acq On : 18 Nov 2021 07:48
Operator : SY/VA
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111721S.M
Title : SW846 8260
Last Update : Thu Nov 18 05:03:38 2021

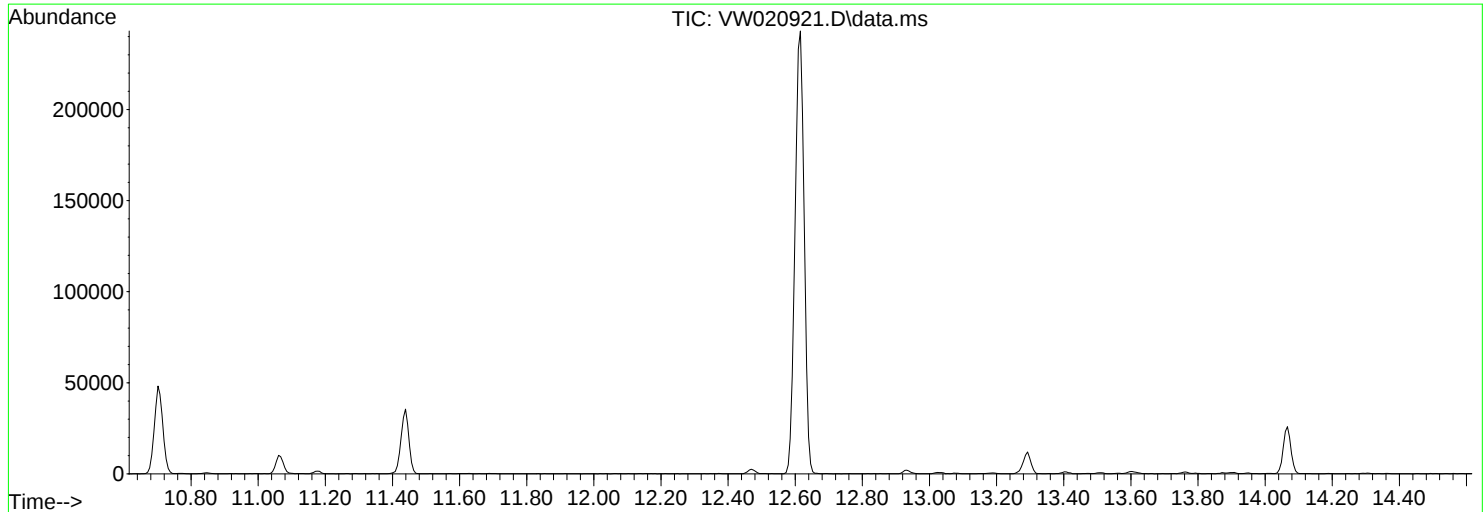

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	5856	PASS
75	95	30	60	50.9	15576	PASS
95	95	100	100	100.0	30587	PASS
96	95	5	9	7.0	2155	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.5	26445	PASS
175	174	5	9	8.7	2308	PASS
176	174	95	101	100.1	26472	PASS
177	176	5	9	8.2	2177	PASS