

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111822\
 Data File : VW025089.D
 Acq On : 18 Nov 2022 10:26
 Operator : SY/VA
 Sample : N5658-10
 Misc : 3.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 19 04:31:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 23:58:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	386814	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	224561	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	29750	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	98438	22.673	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.680%
7) Chloroethane-d5	2.885	69	77585	30.505	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	122.000%
11) 1,1-Dichloroethene-d2	4.019	63	189934	17.562	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.240%
21) 2-Butanone-d5	7.080	46	88938	60.695	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.380%
24) Chloroform-d	7.653	84	328327	27.969	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	111.880%
26) 1,2-Dichloroethane-d4	8.305	65	164007	24.959	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.840%
32) Benzene-d6	8.281	84	600085	41.692	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	166.760%#
36) 1,2-Dichloropropane-d6	9.274	67	201431	47.762	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	191.040%#
41) Toluene-d8	10.323	98	430115	32.098	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	128.400%
43) trans-1,3-Dichloroprop...	10.579	79	52680	28.170	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	112.680%
47) 2-Hexanone-d5	10.927	63	59318	81.423	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	162.840%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	130364	38.713	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	154.840%#
66) 1,2-Dichlorobenzene-d4	13.853	152	31803	27.817	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	111.280%
Target Compounds					Qvalue	
48) 2-Hexanone	10.927	43	7093	5.325	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111822\
Data File : VW025089.D
Acq On : 18 Nov 2022 10:26
Operator : SY/VA
Sample : N5658-10
Misc : 3.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 19 04:31:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 23:58:11 2022
Response via : Initial Calibration

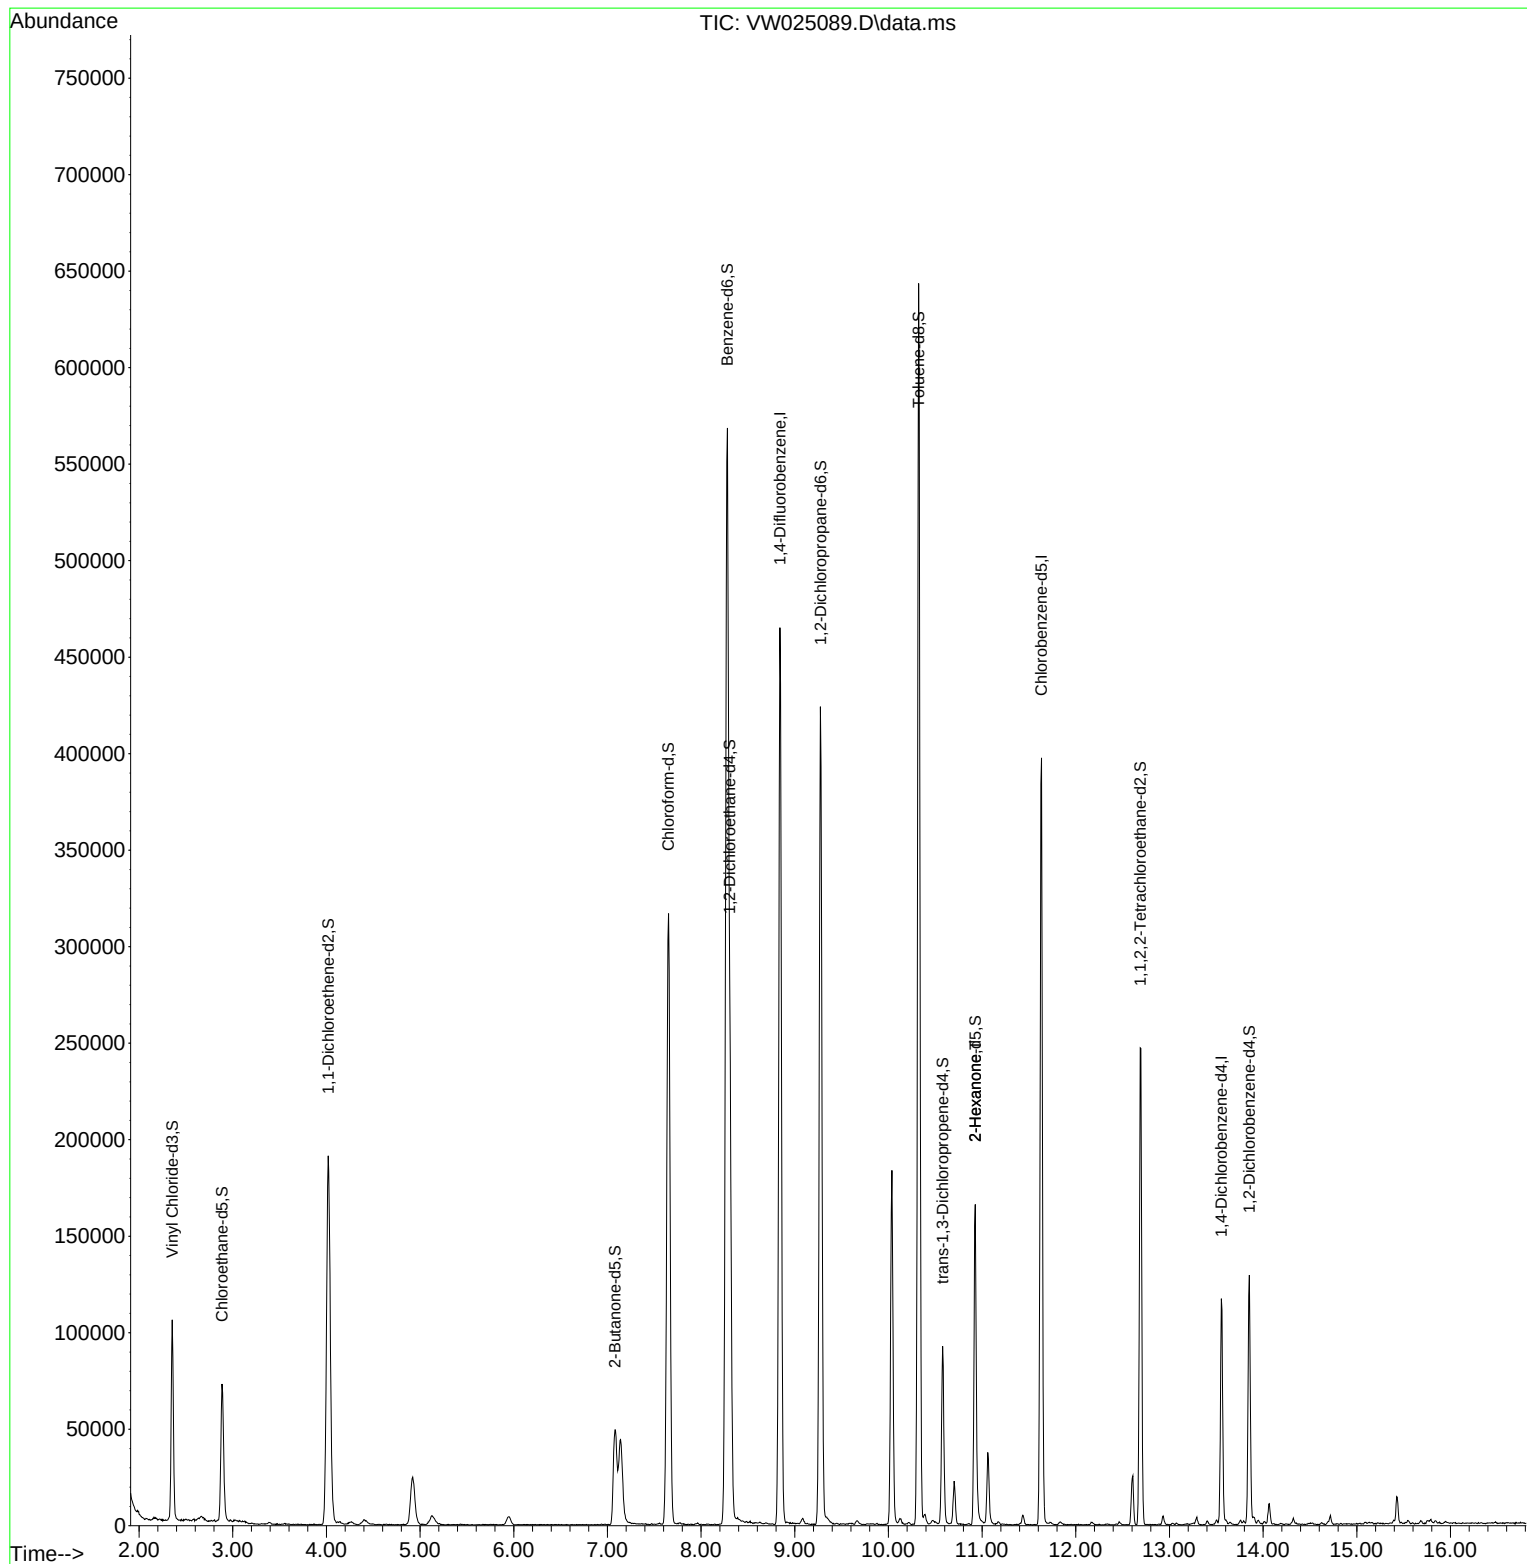

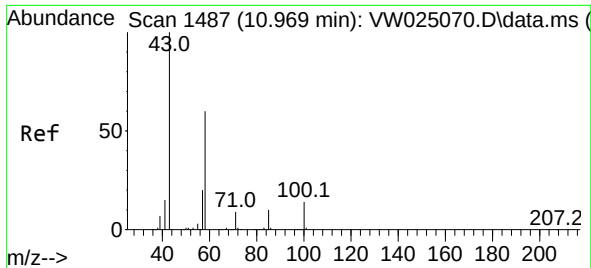

#48
 2-Hexanone
 Concen: 5.325 ug/L
 RT: 10.927 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW025089.D
 Acq: 18 Nov 2022 10:26

Instrument :
 MSVOA_W
 ClientSampleId :

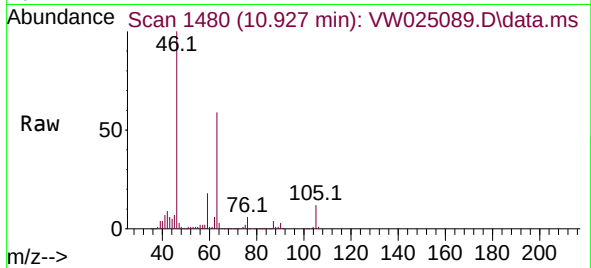

Tgt Ion: 43 Resp: 7093
 Ion Ratio Lower Upper
 43 100
 58 25.1 46.1 69.1#
 57 27.8 16.2 24.2#
 100 1.9 11.0 16.6#

