

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111822\
 Data File : VW025100.D
 Acq On : 18 Nov 2022 16:04
 Operator : SY/VA
 Sample : N5712-07
 Misc : 4.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 19 04:33:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 23:58:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	384442	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	303874	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	98721	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	85536	19.823	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.280%
7) Chloroethane-d5	2.891	69	64930	25.687	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.760%
11) 1,1-Dichloroethene-d2	4.019	63	153499	14.281	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.120%
21) 2-Butanone-d5	7.074	46	86816	59.612	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.220%
24) Chloroform-d	7.653	84	271751	23.292	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.160%
26) 1,2-Dichloroethane-d4	8.305	65	150863	23.100	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.400%
32) Benzene-d6	8.275	84	508020	26.083	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.320%
36) 1,2-Dichloropropane-d6	9.274	67	167389	29.331	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	117.320%
41) Toluene-d8	10.323	98	414424	22.855	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.400%
43) trans-1,3-Dichloroprop...	10.579	79	52568	20.773	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.080%
47) 2-Hexanone-d5	10.927	63	53283	54.049	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.100%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	136506	29.957	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	119.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	90331	23.810	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.240%
Target Compounds						
34) Trichloroethene	8.842	95	11805	2.437	ug/L	Qvalue # 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111822\
Data File : VW025100.D
Acq On : 18 Nov 2022 16:04
Operator : SY/VA
Sample : N5712-07
Misc : 4.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Nov 19 04:33:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 23:58:11 2022
Response via : Initial Calibration

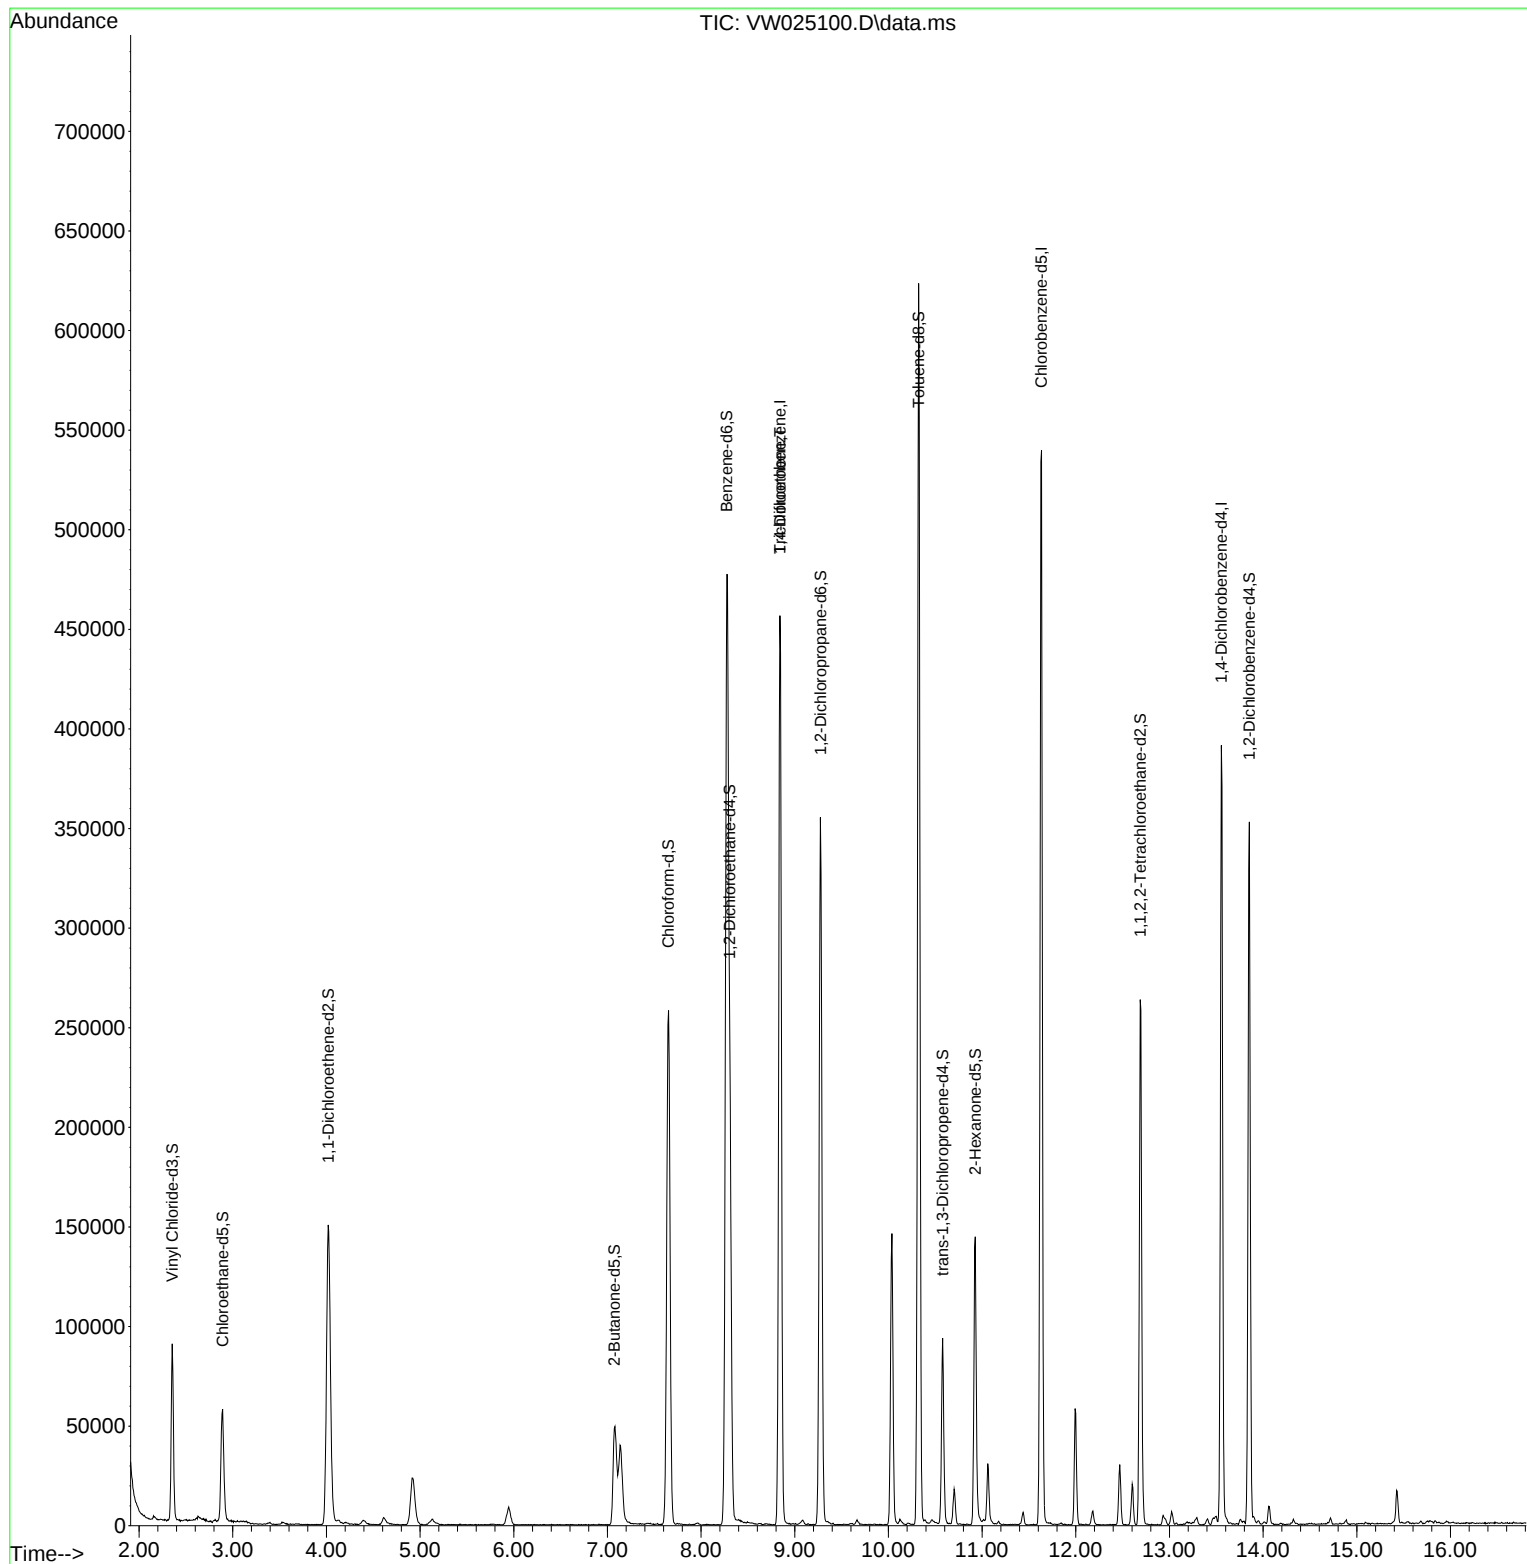

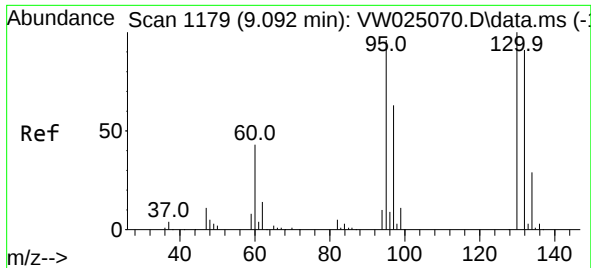

#34
 Trichloroethene
 Concen: 2.437 ug/L
 RT: 8.842 min Scan# 1179
 Delta R.T. -0.250 min
 Lab File: VW025100.D
 Acq: 18 Nov 2022 16:04

Instrument :
 MSVOA_W
 ClientSampleId :

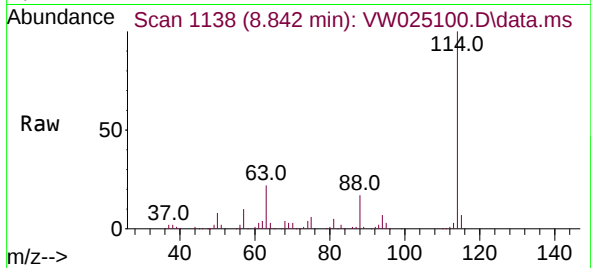

Tgt Ion:	95	Resp:	11805
Ion	Ratio	Lower	Upper
95	100		
97	0.0	44.7	83.1#
132	0.0	62.6	116.2#
130	0.0	69.1	128.3#

