

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111822\
 Data File : VW025103.D
 Acq On : 18 Nov 2022 17:24
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Nov 19 04:34:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 23:58:11 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	434286	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	385653	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	178678	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	91106	18.690	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.760%
7) Chloroethane-d5	2.892	69	69805	24.446	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.800%
11) 1,1-Dichloroethene-d2	4.019	63	178084	14.666	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.680%
21) 2-Butanone-d5	7.080	46	76109	46.262	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.520%
24) Chloroform-d	7.647	84	293910	22.300	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.200%
26) 1,2-Dichloroethane-d4	8.305	65	152003	20.603	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.400%
32) Benzene-d6	8.275	84	581433	23.522	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.080%
36) 1,2-Dichloropropane-d6	9.275	67	180806	24.964	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.840%
41) Toluene-d8	10.323	98	505020	21.945	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.760%
43) trans-1,3-Dichloroprop...	10.579	79	65536	20.406	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.640%
47) 2-Hexanone-d5	10.921	63	56782	45.384	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.760%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	136817	23.658	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.640%
66) 1,2-Dichlorobenzene-d4	13.847	152	164602	23.972	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.880%
Target Compounds						
34) Trichloroethene	8.842	95	13494	2.195	ug/L #	7
37) 1,2-Dichloropropane	9.275	63	20535	3.643	ug/L #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111822\
Data File : VW025103.D
Acq On : 18 Nov 2022 17:24
Operator : SY/VA
Sample : VIBLK
Misc : 5.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Nov 19 04:34:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 23:58:11 2022
Response via : Initial Calibration

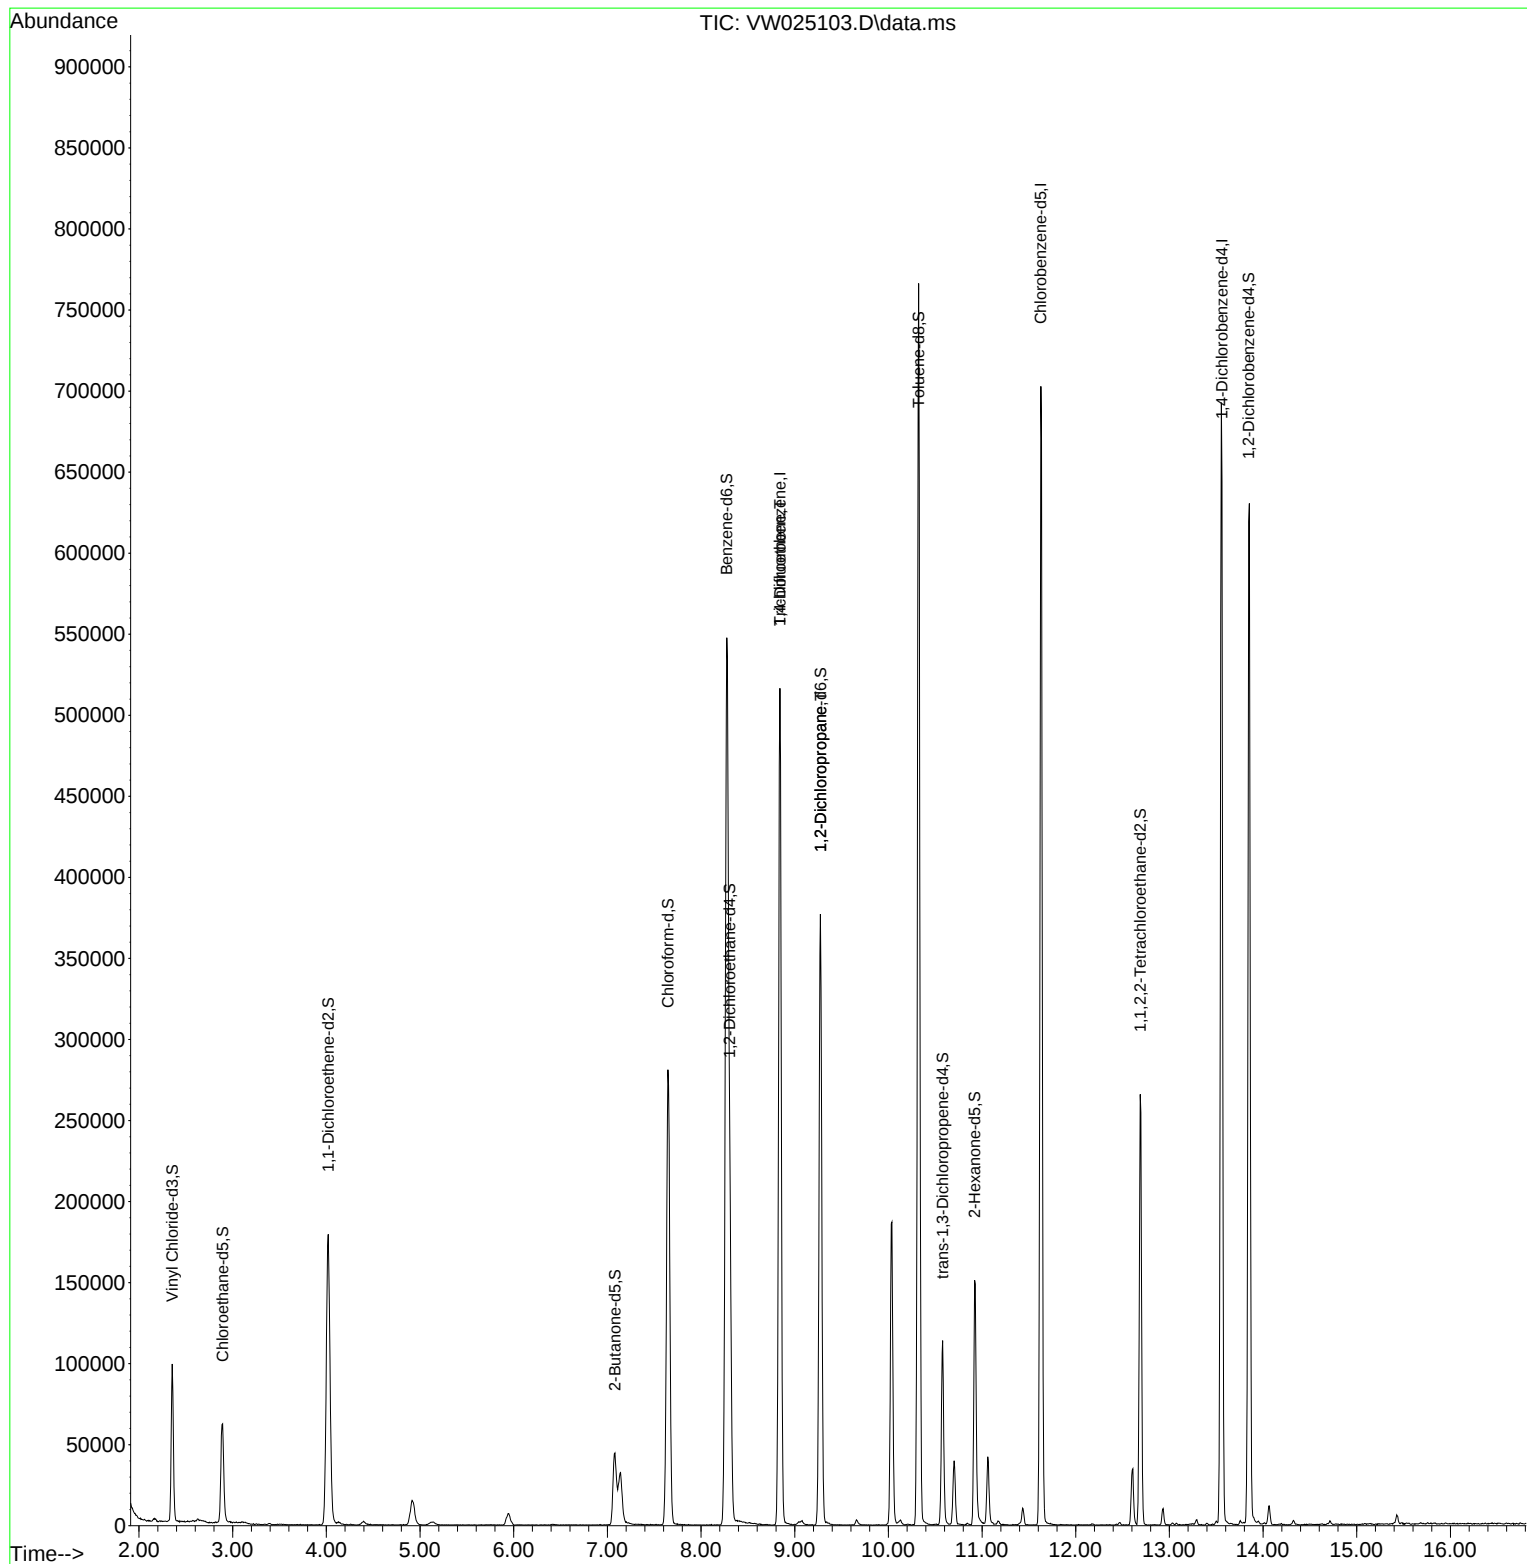

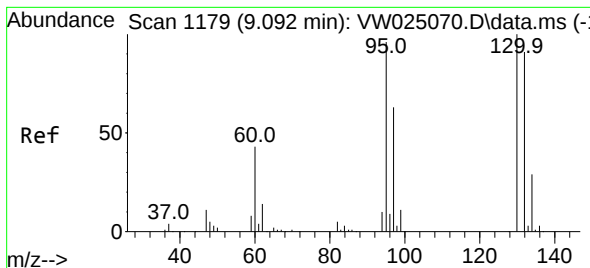

#34

Trichloroethene

Concen: 2.195 ug/L

RT: 8.842 min Scan# 1179

Delta R.T. -0.250 min

Lab File: VW025103.D

Acq: 18 Nov 2022 17:24

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion: 95 Resp: 13494





Ion Ratio Lower Upper

95 100

97 0.0 44.7 83.1#

132 0.0 62.6 116.2#

130 0.0 69.1 128.3#

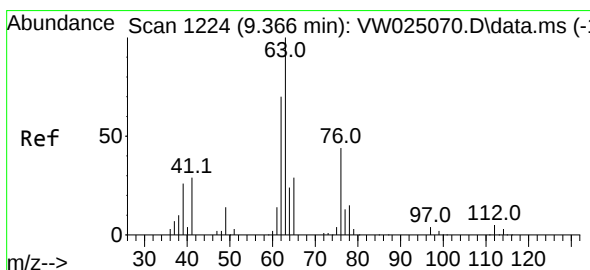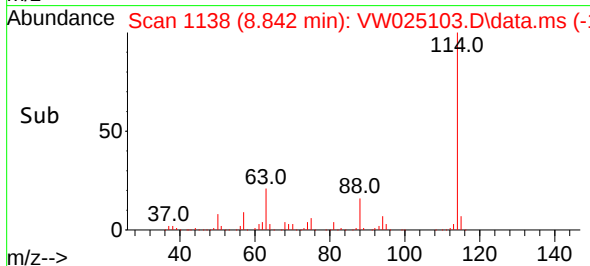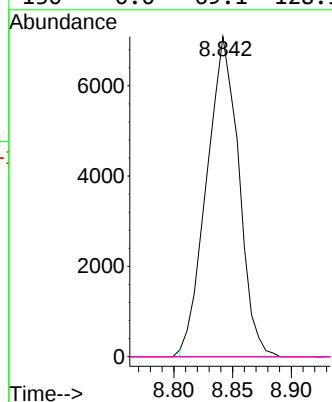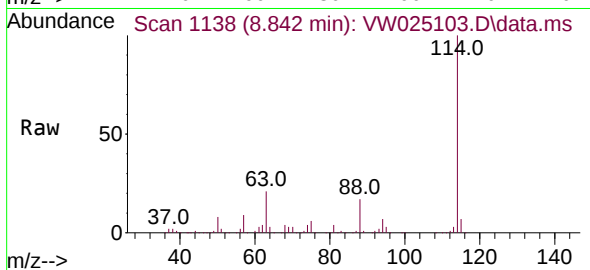

#37

1,2-Dichloropropane

Concen: 3.643 ug/L

RT: 9.275 min Scan# 1209

Delta R.T. -0.091 min

Lab File: VW025103.D

Acq: 18 Nov 2022 17:24

Tgt Ion: 63 Resp: 20535

Ion Ratio Lower Upper

63 100

112 0.2 3.6 5.4#

