

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111822\
 Data File : VW025093.D
 Acq On : 18 Nov 2022 12:24
 Operator : SY/VA
 Sample : N5659-03
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Nov 19 04:32:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Nov 17 23:58:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	408253	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	368498	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	168141	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	82767	18.062	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.240%
7) Chloroethane-d5	2.891	69	62899	23.432	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.720%
11) 1,1-Dichloroethene-d2	4.019	63	157578	13.805	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.200%
21) 2-Butanone-d5	7.080	46	54580	35.292	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.580%
24) Chloroform-d	7.647	84	253383	20.451	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.800%
26) 1,2-Dichloroethane-d4	8.305	65	123469	17.803	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.200%
32) Benzene-d6	8.275	84	506808	21.457	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.840%
36) 1,2-Dichloropropane-d6	9.274	67	152685	22.062	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.240%
41) Toluene-d8	10.323	98	441122	20.061	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.240%
43) trans-1,3-Dichloroprop...	10.579	79	51848	16.896	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.600%
47) 2-Hexanone-d5	10.927	63	41587	34.787	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.580%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	103874	18.798	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	75.200%
66) 1,2-Dichlorobenzene-d4	13.853	152	137603	21.296	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.200%
Target Compounds						
16) Methylene chloride	4.922	84	24424	3.369	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW111822\
Data File : VW025093.D
Acq On : 18 Nov 2022 12:24
Operator : SY/VA
Sample : N5659-03
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Nov 19 04:32:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102622SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Nov 17 23:58:11 2022
Response via : Initial Calibration

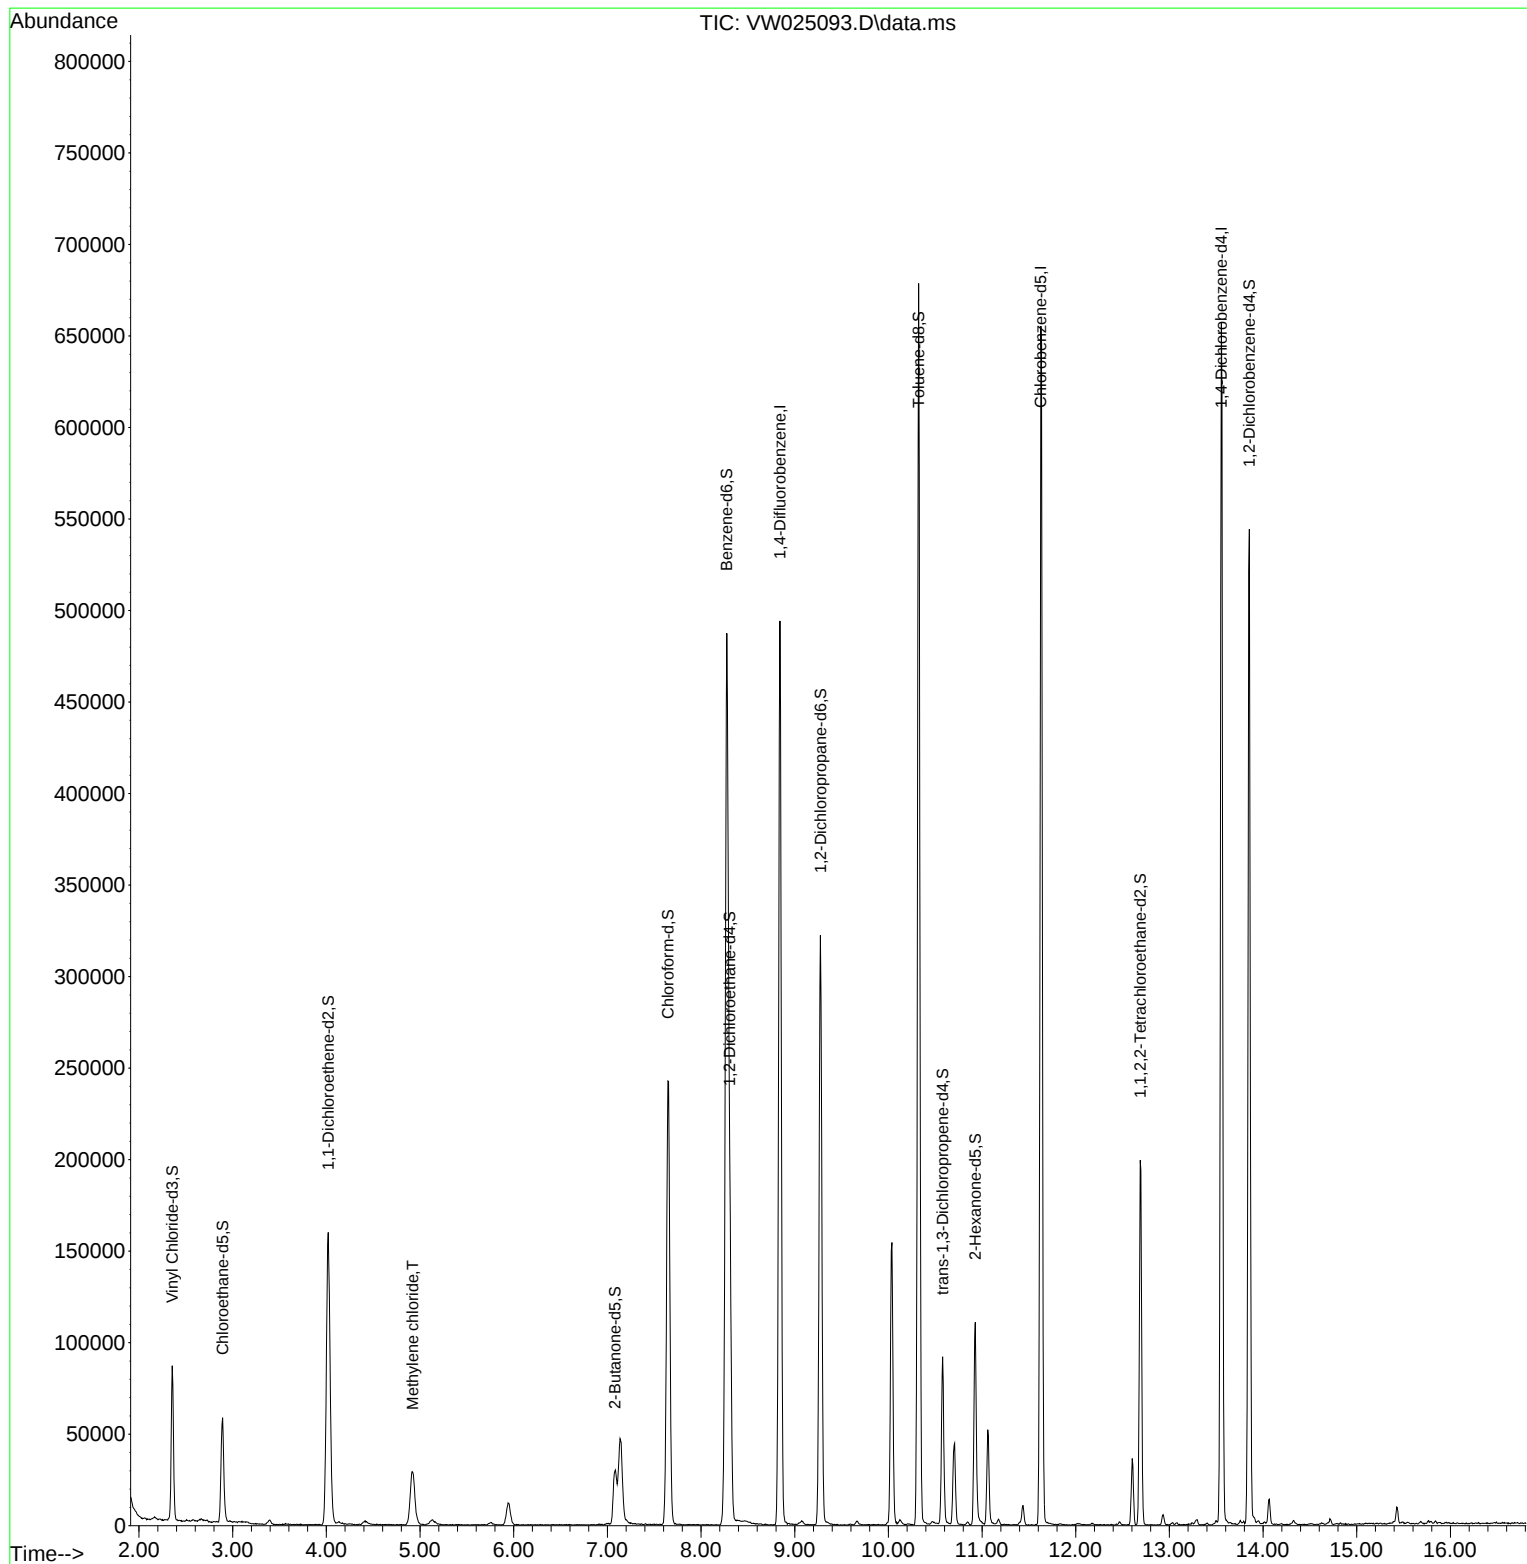

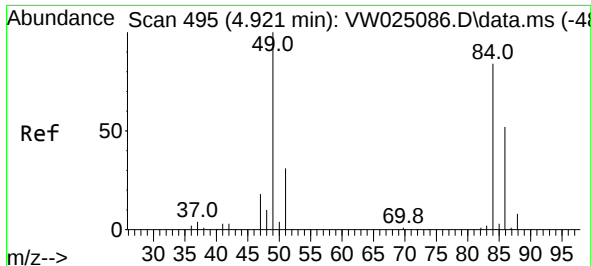

#16

Methylene chloride

Concen: 3.369 ug/L

RT: 4.922 min Scan# 49

Delta R.T. -0.000 min

Lab File: VW025093.D


Acq: 18 Nov 2022 12:24

Instrument :

MSVOA_W

ClientSampleId :

VHBLK001

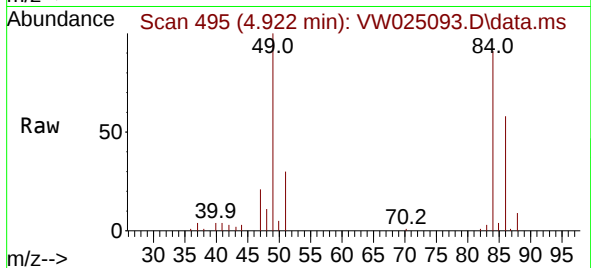

Tgt Ion: 84 Resp: 24424

Ion Ratio Lower Upper

84 100

86 64.2 42.6 79.0

49 110.0 81.9 152.1

