

Data File : VW014083.D
 Acq On : 19 Nov 2019 14:33
 Operator : SY/VA
 Sample : K5845-08
 Misc : 5.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Quant Time: Nov 20 06:03:12 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 20 05:59:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	305252	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	297833	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	167689	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	113812	23.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.48%
7) Chloroethane-d5	2.89	69	91799	23.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.00%
10) 1,1-Dichloroethene-d2	4.01	63	171879	17.20	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.80%
20) 2-Butanone-d5	7.07	46	68372	48.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.64%
24) Chloroform-d	7.65	84	235568	25.10	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	8.31	65	125071	26.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.04%
29) Benzene-d6	8.27	84	505047	23.90	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.60%
33) 1,2-Dichloropropane-d6	9.27	67	150809	24.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.44%
37) Toluene-d8	10.32	98	464574	23.18	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.72%
38) trans-1,3-Dichloropropene-	10.57	79	62504	23.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.32%
39) 2-Hexanone-d5	10.92	63	54502	46.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.86%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	117476	25.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	165437	24.56	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.24%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	13.55	75	17158	5.057	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014083.D
Acq On : 19 Nov 2019 14:33
Operator : SY/VA
Sample : K5845-08
Misc : 5.05G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
VHBLK01

Quant Time: Nov 20 06:03:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 20 05:59:38 2019
Response via : Initial Calibration

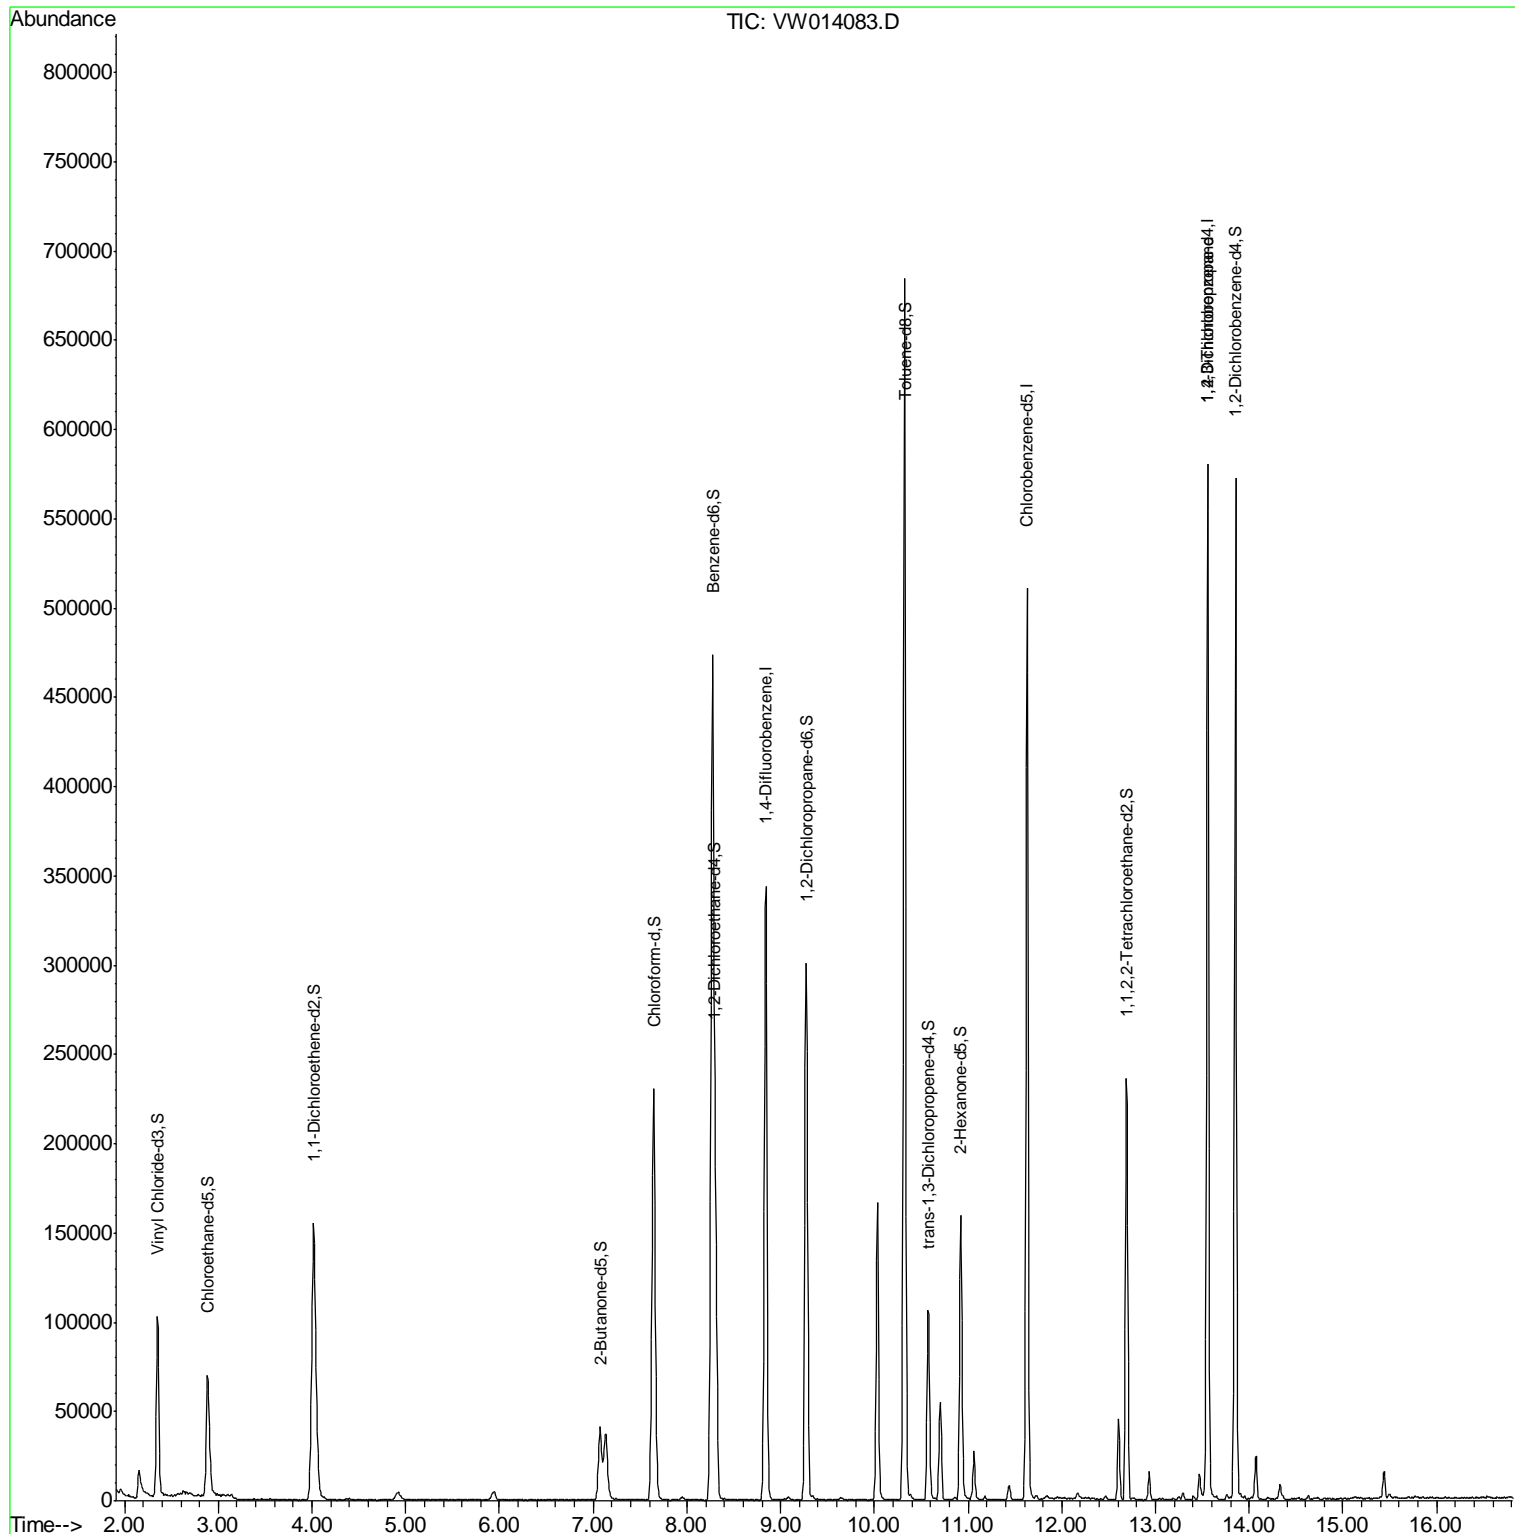

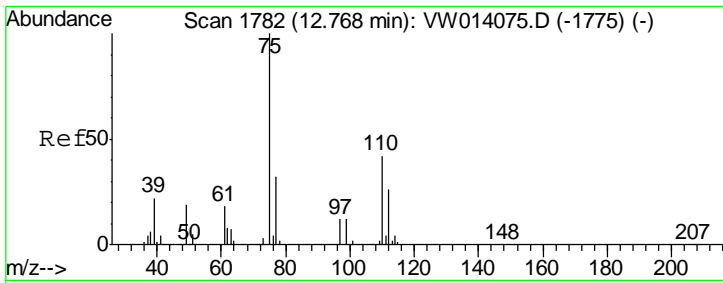

#59
 1,2,3-Trichloropropane
 Concen: 5.057 ug/L
 RT: 13.55 min Scan# 1911
 Delta R.T. 0.79 min
 Lab File: VW014083.D
 Acq: 19 Nov 2019 14:33

Instrument : MSVOA_W
 ClientSampled : VHBLK01

Tgt Ion: 75 Resp: 17158

Ion	Ratio	Lower	Upper
75	100		
77	34.8	25.9	38.9

