

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW111925\  
 Data File : VW032495.D  
 Acq On : 19 Nov 2025 12:30  
 Operator : SY/MD  
 Sample : VIBLK  
 Misc : 5.00g/5mL/MSVOA\_W/SOIL  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 VIBLK

Quant Time: Nov 20 01:17:24 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\82W111025S.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Nov 11 03:48:21 2025  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.965  | 168  | 234404   | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.849  | 114  | 565923   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.629 | 117  | 593417   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.556 | 152  | 281109   | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.319  | 65    | 163095   | 53.969   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 63 - 155 | Recovery | =    | 107.940% |
| 35) Dibromofluoromethane    | 7.904  | 113   | 156598   | 46.217   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 70 - 134 | Recovery | =    | 92.440%  |
| 50) Toluene-d8              | 10.325 | 98    | 555976   | 42.772   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 74 - 123 | Recovery | =    | 85.540%  |
| 62) 4-Bromofluorobenzene    | 12.617 | 95    | 252588   | 51.439   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 17 - 146 | Recovery | =    | 102.880% |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW111925\  
Data File : VW032495.D  
Acq On : 19 Nov 2025 12:30  
Operator : SY/MD  
Sample : VIBLK  
Misc : 5.00g/5mL/MSVOA\_W/SOIL  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VIBLK

Quant Time: Nov 20 01:17:24 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\82W111025S.M  
Quant Title : SW846 8260  
QLast Update : Tue Nov 11 03:48:21 2025  
Response via : Initial Calibration




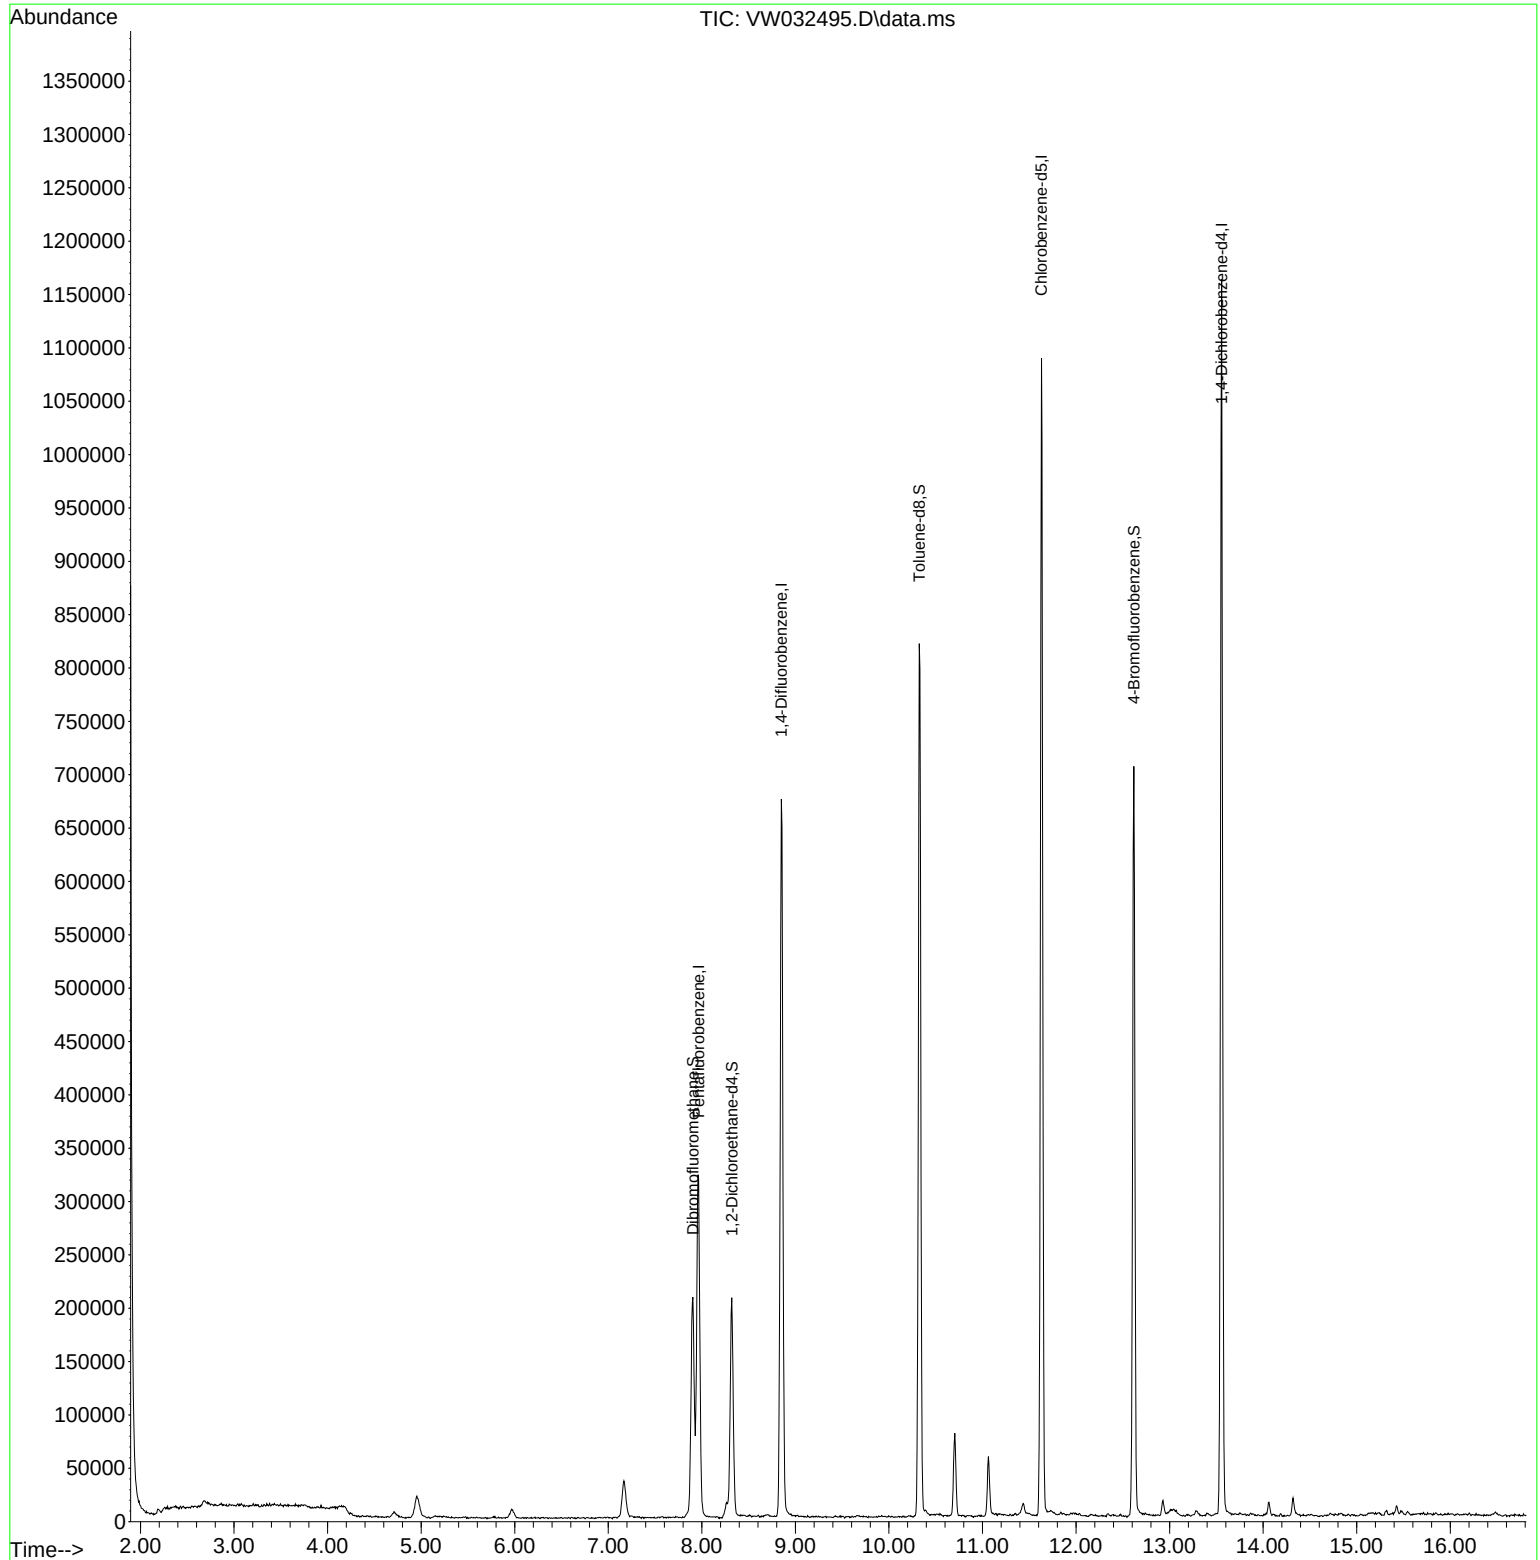


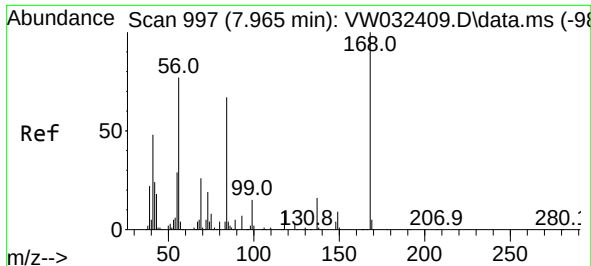

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.965 min Scan# 997  
Delta R.T. 0.000 min  
Lab File: VW032495.D  
Acq: 19 Nov 2025 12:30




Instrument :  
MSVOA\_W  
ClientSampleId :  
VIBLK


Tgt Ion:168 Resp: 234404  
Ion Ratio Lower Upper  
168 100  
99 63.2 45.4 68.2

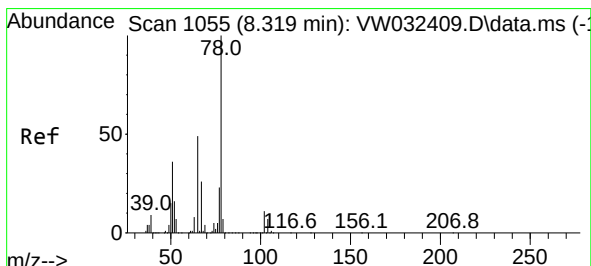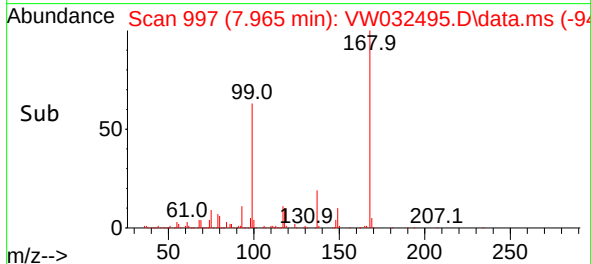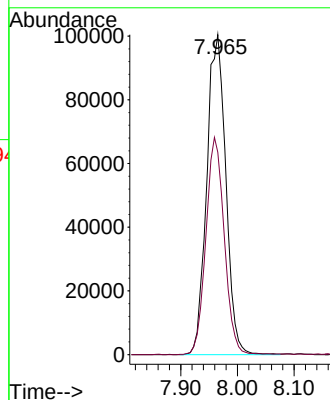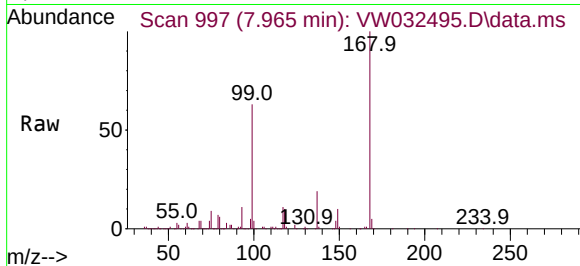

#33  
1,2-Dichloroethane-d4  
Concen: 53.969 ug/l  
RT: 8.319 min Scan# 1055  
Delta R.T. 0.000 min  
Lab File: VW032495.D  
Acq: 19 Nov 2025 12:30

Tgt Ion: 65 Resp: 163095  
Ion Ratio Lower Upper  
65 100  
67 53.9 0.0 106.8


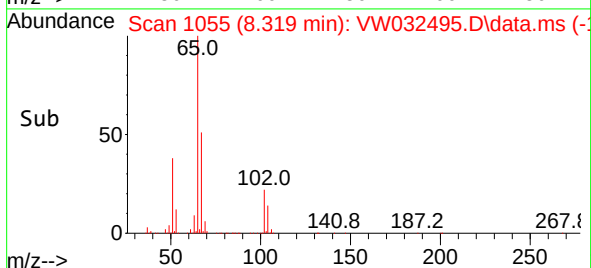
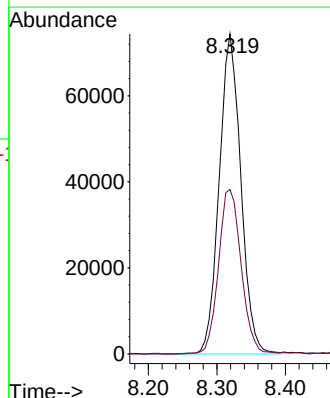
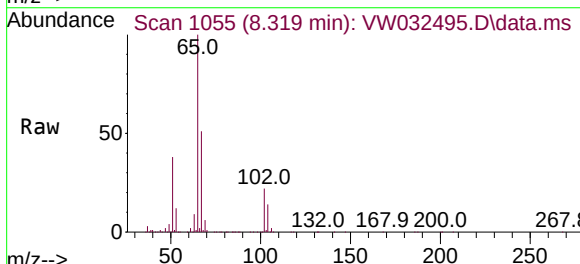


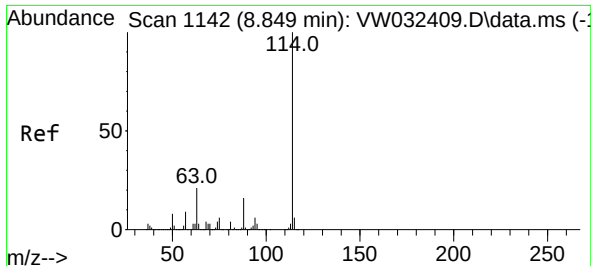

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.849 min Scan# 1142  
Delta R.T. 0.000 min  
Lab File: VW032495.D  
Acq: 19 Nov 2025 12:30




Instrument :  
MSVOA\_W  
ClientSampleId :  
VIBLK


Tgt Ion:114 Resp: 565923  
Ion Ratio Lower Upper  
114 100  
63 22.0 0.0 41.8  
88 16.7 0.0 32.6

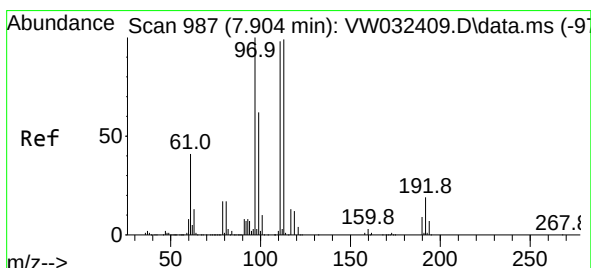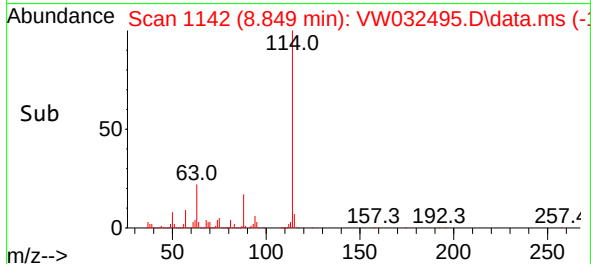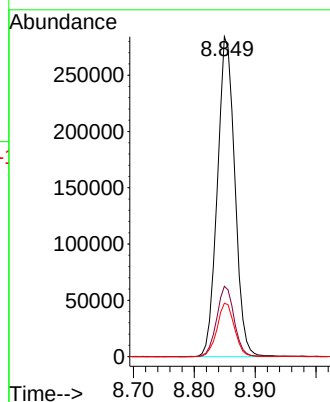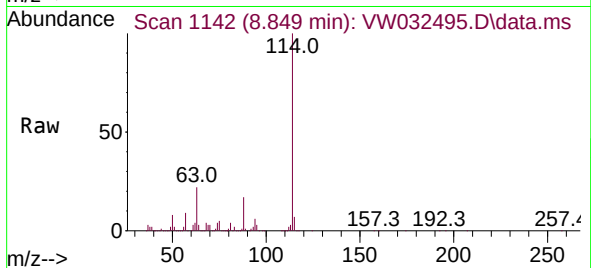

#35  
Dibromofluoromethane  
Concen: 46.217 ug/l  
RT: 7.904 min Scan# 987  
Delta R.T. 0.000 min  
Lab File: VW032495.D  
Acq: 19 Nov 2025 12:30

Tgt Ion:113 Resp: 156598  
Ion Ratio Lower Upper  
113 100  
111 102.9 83.1 124.7  
192 17.7 13.4 20.2


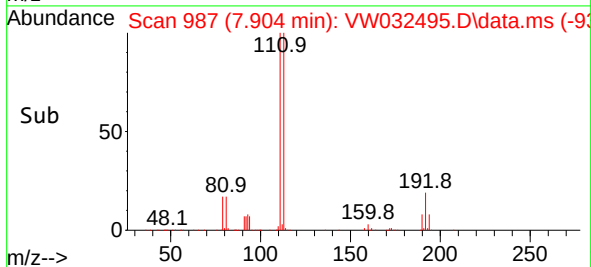
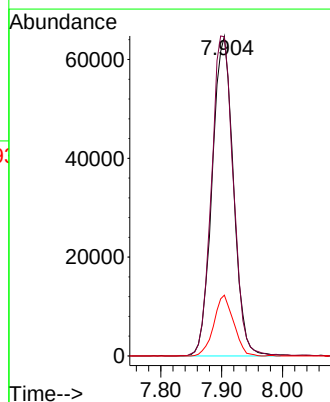
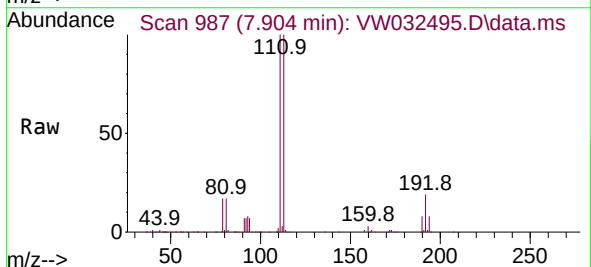


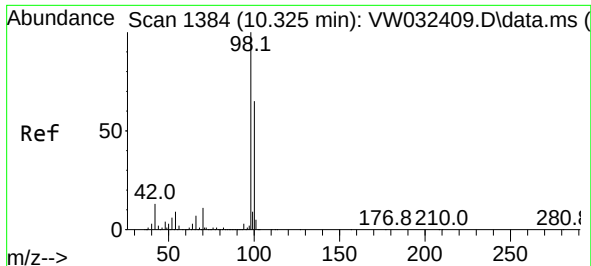

#50  
Toluene-d8  
Concen: 42.772 ug/l  
RT: 10.325 min Scan# 1384  
Delta R.T. 0.000 min  
Lab File: VW032495.D  
Acq: 19 Nov 2025 12:30




Instrument :  
MSVOA\_W  
ClientSampleId :  
VIBLK


Tgt Ion: 98 Resp: 555976  
Ion Ratio Lower Upper  
98 100  
100 67.5 53.3 79.9

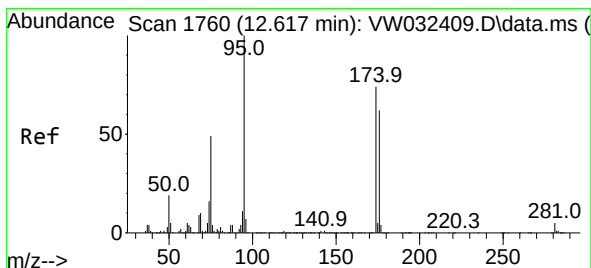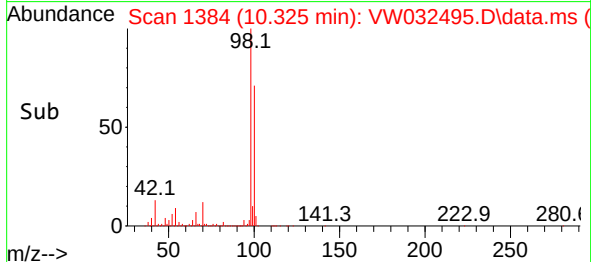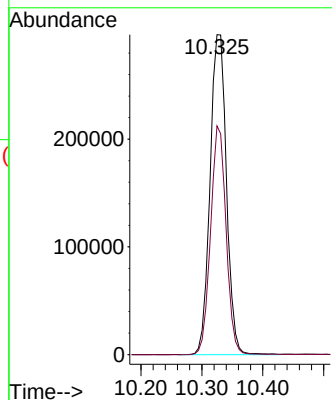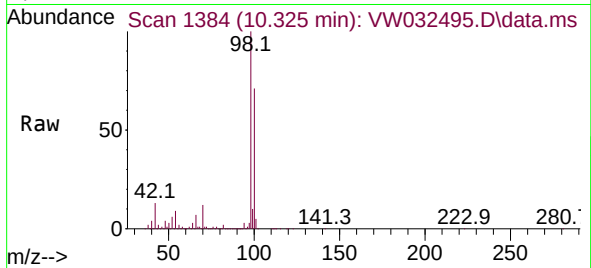

#62  
4-Bromofluorobenzene  
Concen: 51.439 ug/l  
RT: 12.617 min Scan# 1760  
Delta R.T. 0.000 min  
Lab File: VW032495.D  
Acq: 19 Nov 2025 12:30

Tgt Ion: 95 Resp: 252588  
Ion Ratio Lower Upper  
95 100  
174 65.4 0.0 135.4  
176 62.5 0.0 131.8


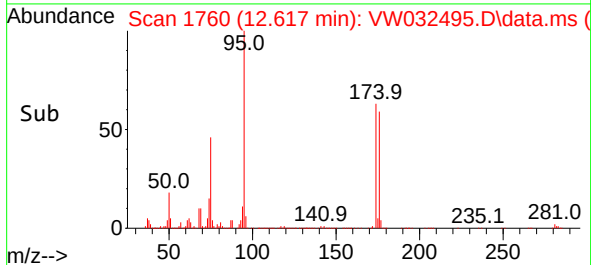
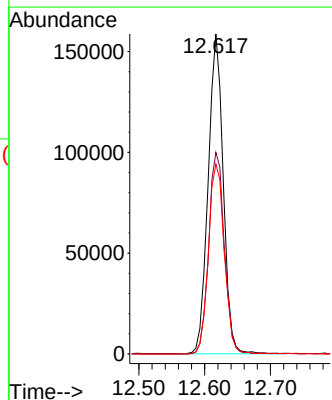
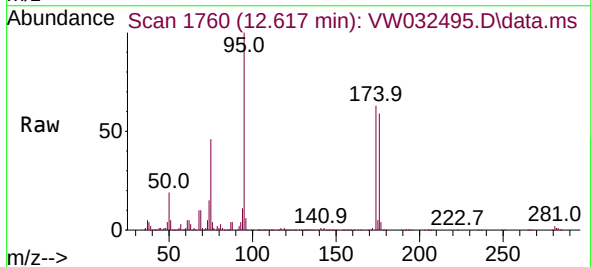


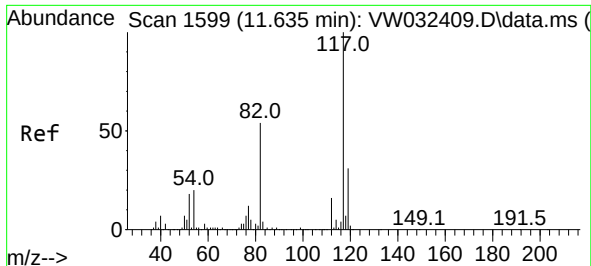

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.629 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: VW032495.D  
Acq: 19 Nov 2025 12:30

Instrument :  
MSVOA\_W  
ClientSampleId :  
VIBLK

Tgt Ion:117 Resp: 593417  
Ion Ratio Lower Upper  
117 100  
82 58.1 43.0 64.4  
119 33.3 25.0 37.6

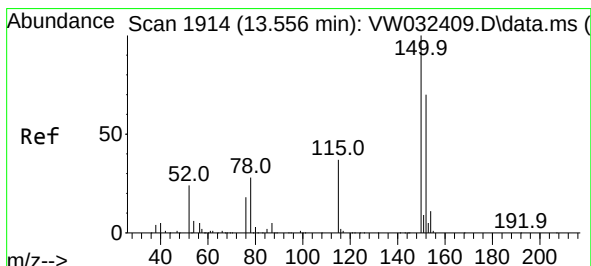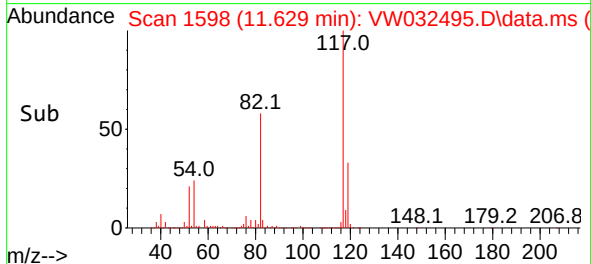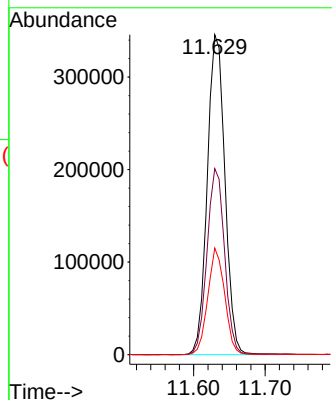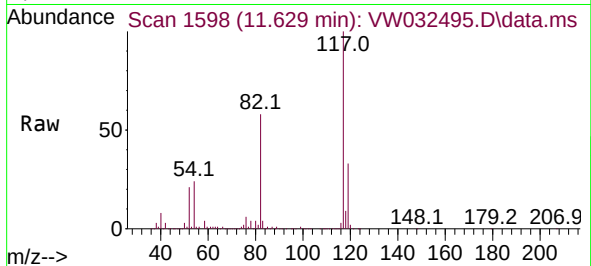

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.556 min Scan# 1914  
Delta R.T. 0.000 min  
Lab File: VW032495.D  
Acq: 19 Nov 2025 12:30

Tgt Ion:152 Resp: 281109  
Ion Ratio Lower Upper  
152 100  
115 64.0 32.8 98.3  
150 158.9 0.0 356.6

