
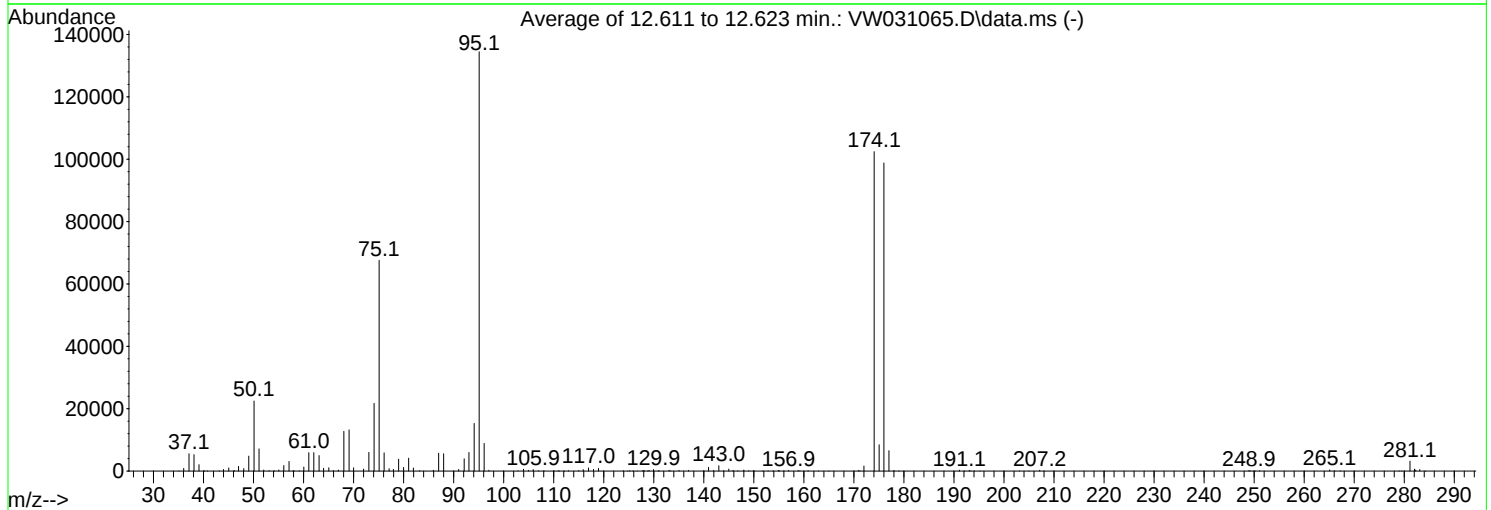


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112024\
Data File : VW031065.D
Acq On : 20 Nov 2024 08:10
Operator : SY/MD
Sample : BFB402
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB402

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112024SMA.M
Title : SFAM01.0
Last Update : Fri Nov 22 00:06:47 2024

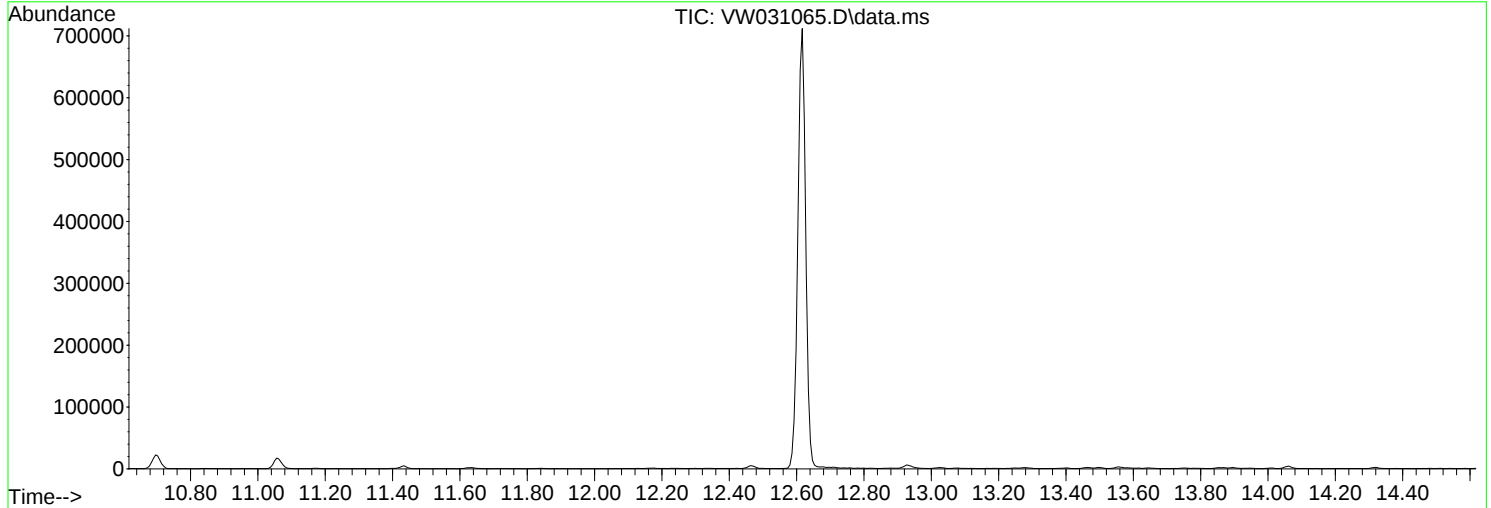

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	22485	PASS
75	95	30	80	50.3	67584	PASS
95	95	100	100	100.0	134472	PASS
96	95	5	9	6.6	8867	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.2	102440	PASS
175	174	5	9	8.2	8436	PASS
176	174	95	101	96.5	98805	PASS
177	176	5	9	6.6	6540	PASS

m/z	Abundance
36.10	278.0
38.20	79.0
40.00	229.0
44.00	214.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

m/z	Abundance
35.10	51.0
36.00	1133.0
37.10	5850.0
38.10	5794.0
39.10	2296.0
39.90	262.0
43.10	112.0
44.00	718.0
45.10	1212.0
46.00	189.0
47.00	1725.0
48.00	883.0
49.10	4991.0
50.10	23680.0
51.10	7677.0
52.00	493.0
53.10	184.0
54.20	124.0
55.10	431.0
56.10	1850.0
57.10	2920.0
57.90	207.0
59.10	119.0
60.00	1369.0
61.00	6580.0
62.10	6044.0
63.10	5598.0
64.00	1094.0
65.00	1289.0
65.90	134.0
67.00	391.0
68.00	13451.0
69.10	14083.0
70.00	974.0
72.00	807.0
73.10	6344.0
74.10	22312.0
75.10	70560.0
76.10	6186.0
77.10	919.0
78.00	517.0
79.00	3853.0
80.00	1258.0
81.00	4425.0
82.00	979.0
83.20	149.0
86.00	358.0
87.00	6096.0
88.00	5308.0
91.00	532.0
92.10	4031.0
93.00	6204.0
94.10	15970.0
95.10	136896.0
96.10	9934.0
97.10	248.0
102.90	175.0
104.00	700.0
105.00	234.0
105.90	551.0
107.10	106.0
108.00	61.0
110.10	71.0
110.90	143.0
112.10	65.0
112.90	155.0
115.10	110.0
115.90	505.0
116.90	1020.0
118.00	589.0
119.00	844.0
124.00	83.0
125.20	335.0
127.80	427.0
129.10	378.0
129.90	552.0
130.90	199.0
133.10	652.0
135.00	194.0
137.00	242.0
140.00	103.0
140.90	1013.0
142.10	207.0
143.00	1746.0
144.00	123.0
145.00	930.0
146.00	292.0
146.80	76.0
148.10	333.0
149.10	146.0
149.90	129.0
152.90	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

154.90	361.0
157.00	240.0
158.80	221.0
159.20	148.0
160.80	161.0
162.90	101.0
165.00	91.0
170.90	384.0
172.00	1686.0
174.00	90544.0
175.10	8234.0
176.00	92168.0
177.00	6606.0
178.00	303.0
179.00	125.0
191.10	500.0
192.10	119.0
193.00	376.0
194.10	115.0
195.20	100.0
203.10	72.0
205.00	102.0
207.10	472.0
208.00	61.0
248.90	363.0
249.20	383.0
250.20	86.0
251.10	194.0
265.10	536.0
266.10	145.0
267.20	198.0
279.00	91.0
279.50	66.0
281.20	5384.0
282.10	1627.0
283.20	704.0
284.30	82.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

m/z	Abundance
36.10	1258.0
37.10	6340.0
38.10	5694.0
39.10	2276.0
40.20	275.0
40.80	82.0
43.20	56.0
44.10	812.0
45.00	1012.0
46.20	177.0
47.00	1830.0
48.10	890.0
49.10	5647.0
50.10	25280.0
51.10	7724.0
52.10	297.0
53.10	147.0
54.20	77.0
54.90	297.0
56.00	2220.0
57.10	3503.0
57.90	165.0
59.20	113.0
60.00	1497.0
61.10	6281.0
62.10	6657.0
63.10	5443.0
64.00	846.0
65.10	1154.0
66.00	106.0
66.90	420.0
68.10	14600.0
69.10	14481.0
70.00	1090.0
72.00	674.0
73.00	6558.0
74.10	24392.0
75.10	74872.0
76.10	6326.0
77.10	824.0
77.90	645.0
79.00	4171.0
80.00	1386.0
81.00	4525.0
81.90	1071.0
83.20	127.0
86.00	203.0
87.00	5967.0
88.00	6580.0
91.00	564.0
92.10	4236.0
93.10	6739.0
94.10	16384.0
95.10	146240.0
96.10	9517.0
97.00	291.0
102.80	114.0
104.00	577.0
105.00	240.0
105.90	457.0
107.10	85.0
108.10	90.0
110.10	75.0
110.90	144.0
112.10	51.0
113.00	85.0
114.90	172.0
116.00	525.0
117.00	987.0
117.90	683.0
119.00	944.0
123.80	95.0
124.80	58.0
125.30	106.0
125.80	84.0
126.70	55.0
128.10	429.0
129.00	303.0
130.00	474.0
131.10	198.0
132.90	161.0
133.40	141.0
135.10	189.0
136.90	245.0
140.00	120.0
141.00	1465.0
141.90	185.0
143.00	1977.0
144.00	152.0
145.00	602.0
145.80	212.0
146.80	163.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

147.90	441.0
149.00	184.0
150.10	101.0
151.80	75.0
152.80	84.0
153.80	114.0
155.10	341.0
156.00	57.0
156.90	298.0
158.90	228.0
160.90	133.0
171.20	300.0
172.00	1902.0
174.10	120600.0
175.10	9747.0
176.00	109848.0
177.00	7366.0
178.00	144.0
179.00	98.0
191.10	322.0
193.10	274.0
203.10	70.0
207.20	274.0
249.00	169.0
249.80	76.0
251.10	99.0
265.10	478.0
266.10	131.0
281.10	2907.0
282.30	755.0
283.00	493.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

m/z	Abundance
36.00	1010.0
37.10	4500.0
38.10	4610.0
39.10	1633.0
39.90	394.0
44.10	673.0
45.10	831.0
46.20	164.0
47.00	1001.0
48.10	691.0
49.00	3781.0
50.10	18496.0
51.10	5980.0
52.10	236.0
53.10	149.0
54.10	79.0
55.10	354.0
56.00	1304.0
57.10	2823.0
58.10	158.0
60.10	1009.0
61.10	4879.0
62.00	5027.0
63.10	3921.0
64.00	717.0
65.10	775.0
66.00	168.0
67.00	278.0
68.10	10170.0
69.10	11045.0
70.00	1062.0
72.10	483.0
73.00	5099.0
74.10	18400.0
75.10	57320.0
76.10	5078.0
77.20	566.0
78.00	539.0
79.00	3469.0
80.00	902.0
81.00	3489.0
82.00	922.0
83.20	93.0
85.80	187.0
87.00	5119.0
88.00	4749.0
91.00	469.0
92.10	3541.0
93.10	5007.0
94.10	13488.0
95.10	120280.0
96.10	7151.0
97.00	283.0
103.90	487.0
104.80	241.0
105.90	474.0
106.90	153.0
108.10	74.0
110.00	89.0
111.10	120.0
112.90	87.0
115.00	173.0
115.80	424.0
117.00	995.0
117.90	363.0
118.90	786.0
125.90	55.0
128.00	332.0
128.80	183.0
129.90	480.0
131.00	120.0
133.00	83.0
135.00	318.0
137.00	230.0
141.00	1193.0
141.80	66.0
143.00	1448.0
144.00	123.0
145.00	437.0
145.70	219.0
148.00	292.0
148.90	89.0
150.00	138.0
152.90	71.0
153.90	137.0
154.90	302.0
156.00	63.0
157.00	145.0
158.90	165.0
160.80	89.0
170.90	213.0
172.00	1313.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402

174.00	96176.0
175.00	7327.0
176.00	94400.0
177.00	5647.0
178.00	180.0
191.00	68.0
192.90	95.0
193.40	88.0
207.20	108.0
251.10	60.0
265.10	171.0
281.20	1332.0
281.90	290.0
282.30	278.0
283.20	296.0

Instrument :
MSVOA_W
ClientSampleId :
BFB402