
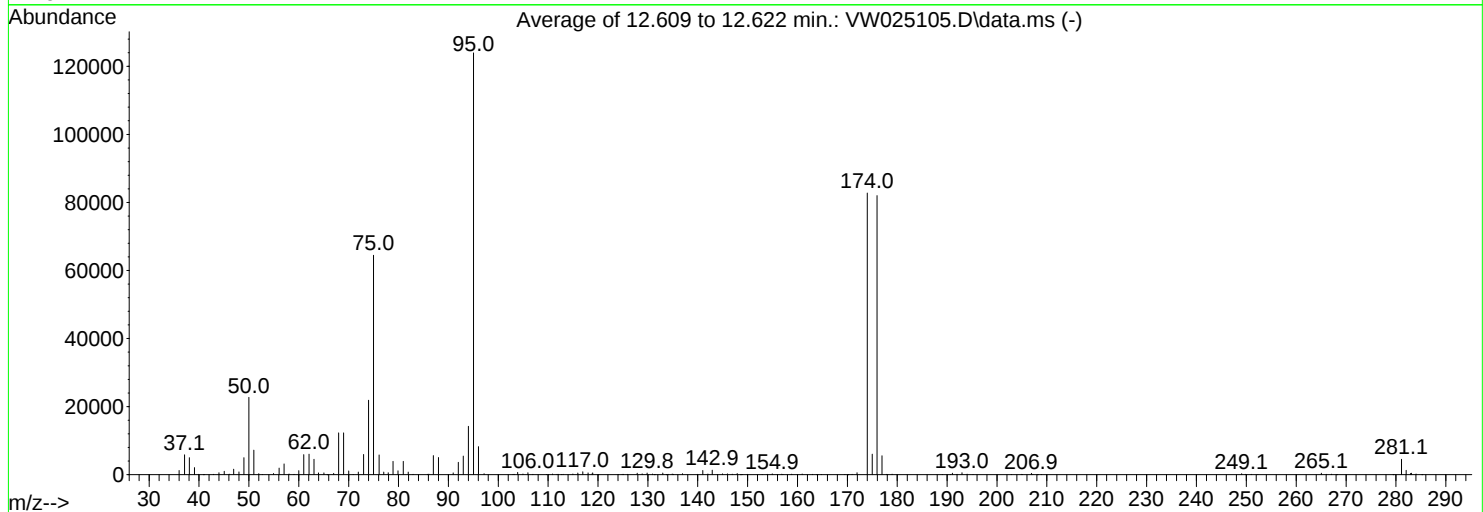


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112122\
Data File : VW025105.D
Acq On : 21 Nov 2022 07:24
Operator : SY/VA
Sample : BFB460
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB460

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112122SMA.M
Title : SFAM01.0
Last Update : Wed Nov 23 04:05:02 2022

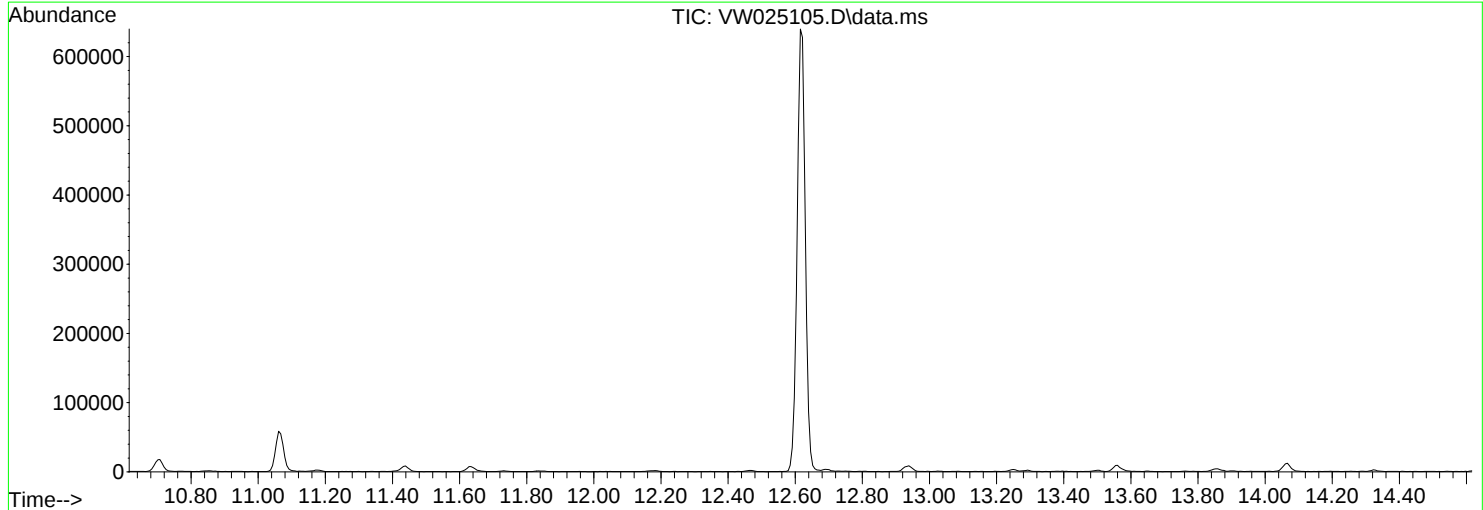

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	22707	PASS
75	95	30	80	52.0	64459	PASS
95	95	100	100	100.0	123971	PASS
96	95	5	9	6.6	8208	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	66.8	82787	PASS
175	174	5	9	7.3	6030	PASS
176	174	95	105	99.1	82032	PASS
177	176	5	10	6.8	5545	PASS

Scan 1749 (12.567 min): VW025105.D\data.ms
BFB460

m/z	Abundance
39.90	261.0
42.90	64.0
44.00	284.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
36.00	1258.0
37.10	4863.0
38.00	4327.0
39.10	1872.0
40.00	315.0
43.00	180.0
44.00	645.0
45.00	1009.0
46.00	141.0
47.00	1508.0
48.00	577.0
49.00	4522.0
50.00	20000.0
51.00	6750.0
52.00	250.0
54.90	283.0
56.00	1616.0
57.10	2365.0
58.00	219.0
59.00	131.0
60.00	867.0
61.00	4982.0
62.00	5423.0
63.00	3998.0
63.90	420.0
65.00	598.0
67.00	201.0
68.00	10373.0
69.00	10737.0
70.00	857.0
70.90	86.0
72.00	604.0
73.00	5543.0
74.00	18584.0
75.00	54024.0
76.10	4928.0
77.10	718.0
77.90	435.0
78.90	3329.0
79.90	1134.0
80.90	3255.0
82.00	507.0
86.10	219.0
87.00	4578.0
88.00	4194.0
91.00	425.0
92.00	3088.0
93.00	4367.0
94.00	11733.0
95.10	103496.0
96.00	6556.0
97.10	269.0
103.20	265.0
103.90	530.0
104.90	198.0
106.00	483.0
107.00	87.0
110.10	68.0
111.00	240.0
111.80	96.0
112.10	118.0
115.00	153.0
116.10	333.0
116.90	788.0
118.10	466.0
118.80	780.0
124.80	236.0
126.10	77.0
127.90	305.0
128.90	238.0
129.80	298.0
131.00	142.0
133.00	732.0
134.00	156.0
134.90	261.0
136.90	155.0
140.00	70.0
141.00	898.0
142.10	111.0
142.90	1289.0
143.90	58.0
145.00	159.0
146.00	262.0
147.00	147.0
147.90	224.0
148.60	52.0
150.00	72.0
153.90	72.0
154.90	239.0
156.80	240.0
158.80	139.0
161.00	149.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

163.10	85.0
164.80	125.0
171.00	58.0
171.90	409.0
174.00	59664.0
175.00	4607.0
175.90	60640.0
177.00	4456.0
178.00	168.0
178.90	193.0
189.00	97.0
191.00	786.0
192.00	142.0
193.00	829.0
194.10	192.0
195.20	112.0
202.90	104.0
204.90	230.0
206.90	669.0
208.10	65.0
208.90	102.0
249.00	491.0
249.80	103.0
250.10	96.0
251.10	193.0
252.30	83.0
265.00	609.0
266.10	92.0
267.10	199.0
279.40	76.0
281.10	6570.0
282.00	1736.0
282.90	1035.0
284.10	242.0
285.20	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
36.10	1304.0
37.10	6258.0
38.10	5564.0
39.10	2189.0
40.00	361.0
40.90	56.0
42.90	152.0
44.00	910.0
45.10	1056.0
46.10	132.0
47.00	1734.0
48.00	903.0
49.00	5414.0
50.00	24552.0
51.00	7906.0
52.00	364.0
55.00	339.0
56.00	2461.0
57.00	3886.0
58.10	211.0
59.10	90.0
60.00	1464.0
61.00	6677.0
62.10	6399.0
63.00	4806.0
64.00	700.0
65.10	516.0
67.00	508.0
68.00	13757.0
69.00	13542.0
70.00	1309.0
70.90	51.0
71.90	784.0
73.00	6424.0
74.00	23216.0
75.00	71600.0
76.10	6418.0
77.10	845.0
78.00	659.0
78.90	3974.0
79.90	1242.0
81.00	4398.0
81.90	840.0
82.90	89.0
85.80	279.0
87.00	6059.0
88.00	5009.0
90.90	654.0
92.00	3673.0
93.00	6107.0
94.00	15536.0
95.00	136768.0
96.10	9460.0
97.20	300.0
102.90	158.0
103.90	749.0
105.00	196.0
105.90	564.0
106.90	100.0
109.70	97.0
110.10	101.0
110.80	172.0
112.00	143.0
112.70	119.0
113.10	143.0
115.00	235.0
115.90	547.0
117.00	979.0
118.00	559.0
119.00	791.0
120.00	51.0
124.10	102.0
125.10	224.0
125.90	164.0
127.90	538.0
128.90	246.0
129.90	533.0
131.00	305.0
133.10	480.0
134.10	74.0
135.10	346.0
137.00	323.0
140.00	96.0
141.00	1472.0
142.00	193.0
142.90	1309.0
144.90	325.0
145.90	216.0
146.80	174.0
147.90	389.0
149.00	97.0
149.90	89.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

152.90	128.0
154.00	114.0
155.00	192.0
157.10	221.0
158.90	108.0
161.00	208.0
163.00	101.0
164.80	67.0
169.50	53.0
170.80	82.0
172.00	700.0
174.00	90176.0
175.00	6362.0
176.00	91464.0
177.00	6327.0
177.80	114.0
179.00	194.0
189.10	104.0
191.10	448.0
192.00	70.0
193.00	535.0
194.00	108.0
205.10	152.0
206.90	184.0
207.20	236.0
208.90	54.0
249.10	224.0
249.80	90.0
250.90	138.0
265.10	349.0
266.10	215.0
267.00	154.0
268.10	64.0
281.10	4396.0
282.10	1315.0
283.10	887.0
284.00	165.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

m/z	Abundance
35.90	1075.0
37.10	6369.0
38.00	5010.0
39.10	2210.0
39.90	336.0
43.00	114.0
44.00	950.0
45.10	971.0
46.10	195.0
46.90	1504.0
48.00	923.0
49.00	5090.0
50.00	23568.0
51.00	6970.0
52.00	298.0
52.70	94.0
55.00	308.0
56.10	1765.0
57.00	3166.0
58.00	151.0
59.00	66.0
60.00	1188.0
61.00	6009.0
62.10	6304.0
63.10	4732.0
64.00	436.0
65.10	462.0
65.70	55.0
67.00	449.0
68.00	12714.0
69.00	12574.0
70.00	1117.0
72.00	903.0
73.00	5879.0
74.00	23840.0
75.00	67752.0
76.10	5972.0
77.00	773.0
78.00	655.0
78.90	4394.0
79.90	971.0
80.90	4114.0
81.90	932.0
82.90	149.0
86.10	188.0
87.00	6196.0
88.00	5950.0
90.90	526.0
92.00	4147.0
93.00	5855.0
94.00	15341.0
95.00	131648.0
96.10	8608.0
97.10	317.0
103.00	103.0
103.90	664.0
104.90	196.0
105.90	638.0
106.90	106.0
109.70	74.0
110.90	137.0
111.80	188.0
112.90	162.0
114.90	183.0
115.90	550.0
116.90	820.0
117.90	585.0
118.90	722.0
124.00	107.0
124.90	92.0
125.10	92.0
125.90	66.0
127.80	389.0
128.80	193.0
129.80	536.0
130.80	138.0
131.30	70.0
132.90	259.0
133.70	59.0
134.90	285.0
136.90	317.0
139.90	111.0
141.00	1294.0
142.10	256.0
142.90	1328.0
144.00	66.0
144.90	180.0
146.00	201.0
146.90	71.0
147.90	360.0
149.00	117.0
149.90	156.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460

152.90	81.0
153.90	77.0
154.90	288.0
156.00	148.0
156.90	160.0
158.90	209.0
160.80	167.0
162.90	70.0
163.90	65.0
169.50	71.0
170.10	67.0
171.00	106.0
171.90	562.0
174.00	98520.0
175.00	7120.0
176.00	93992.0
176.90	5853.0
178.10	201.0
179.00	78.0
190.70	153.0
192.00	77.0
193.00	340.0
193.90	71.0
207.00	264.0
248.90	138.0
249.90	64.0
265.00	279.0
267.00	75.0
281.10	2617.0
282.10	766.0
283.10	369.0
284.10	209.0

Instrument :
MSVOA_W
ClientSampleId :
BFB460