

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW112219\
Quantitation Report (Qedit)




Data File : VW014097.D
Acq On : 22 Nov 2019 16:06
Operator : SY/VA
Sample : K5989-07
Misc : 4.90G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BK3

Manual Integrations
APPROVED

MMDadoda
11/26/2019 1:35:38 AM

Quant Time: Nov 22 23:04:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 22 23:01:18 2019
Response via : Initial Calibration

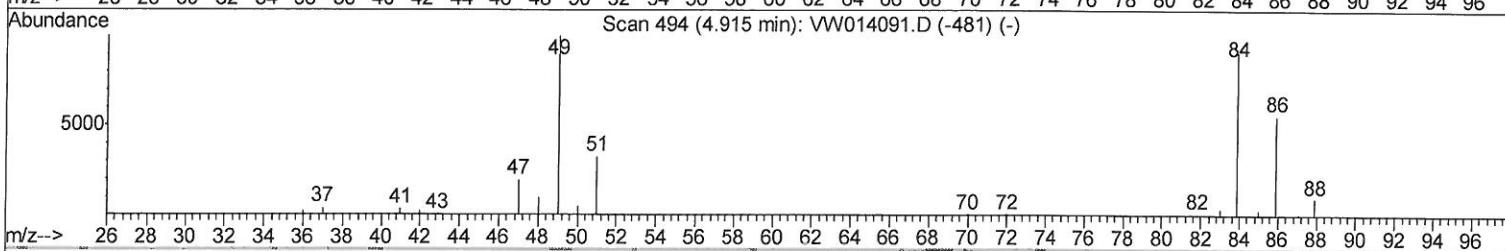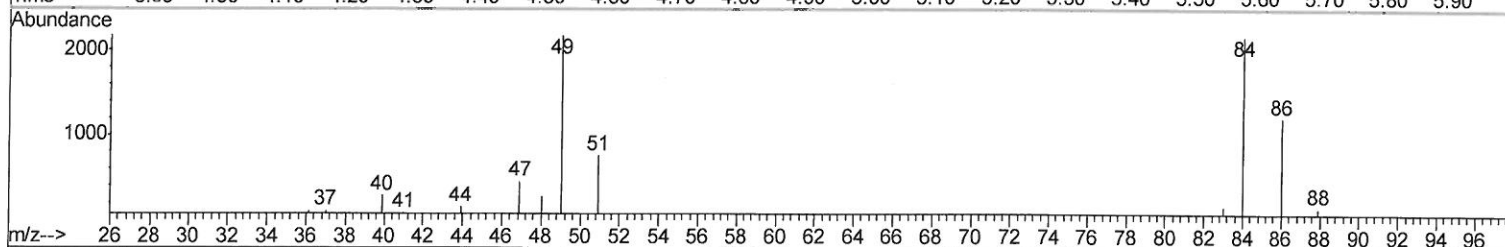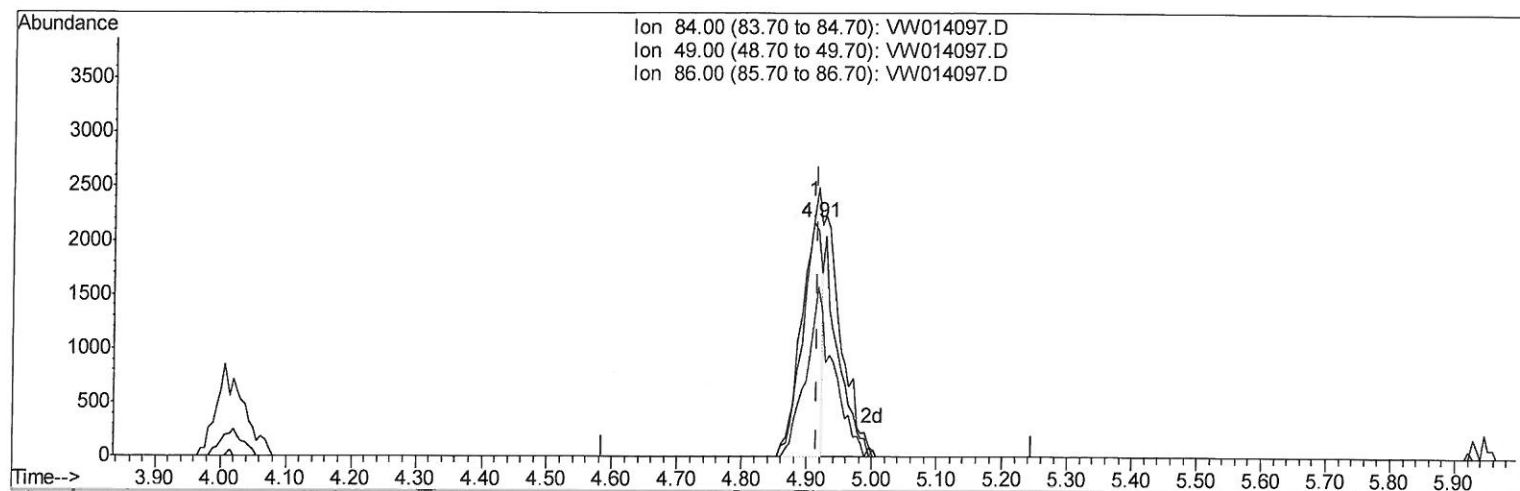

TIC: VW014097.D

(16) Methylene chloride (T)

4.909min (-0.006) 0.96ug/L

response 4501

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	100.46
86.00	62.40	55.61
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW112219\
Quantitation Report (Qedit)




Data File : VW014097.D
Acq On : 22 Nov 2019 16:06
Operator : SY/VA
Sample : K5989-07
Misc : 4.90G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BK3

Manual Integrations
APPROVED

MMDadoda
11/26/2019 1:35:38 AM

Quant Time: Nov 22 23:04:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 22 23:01:18 2019
Response via : Initial Calibration

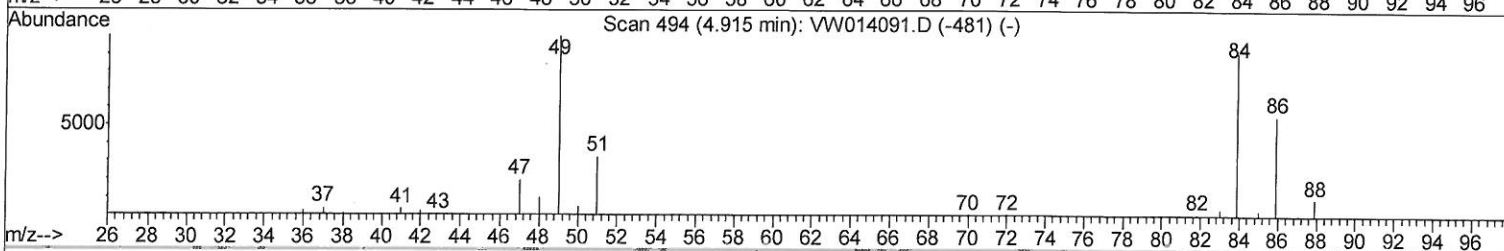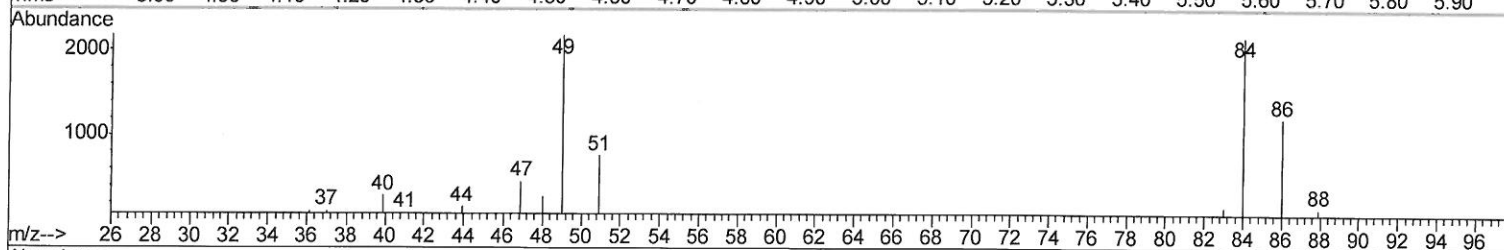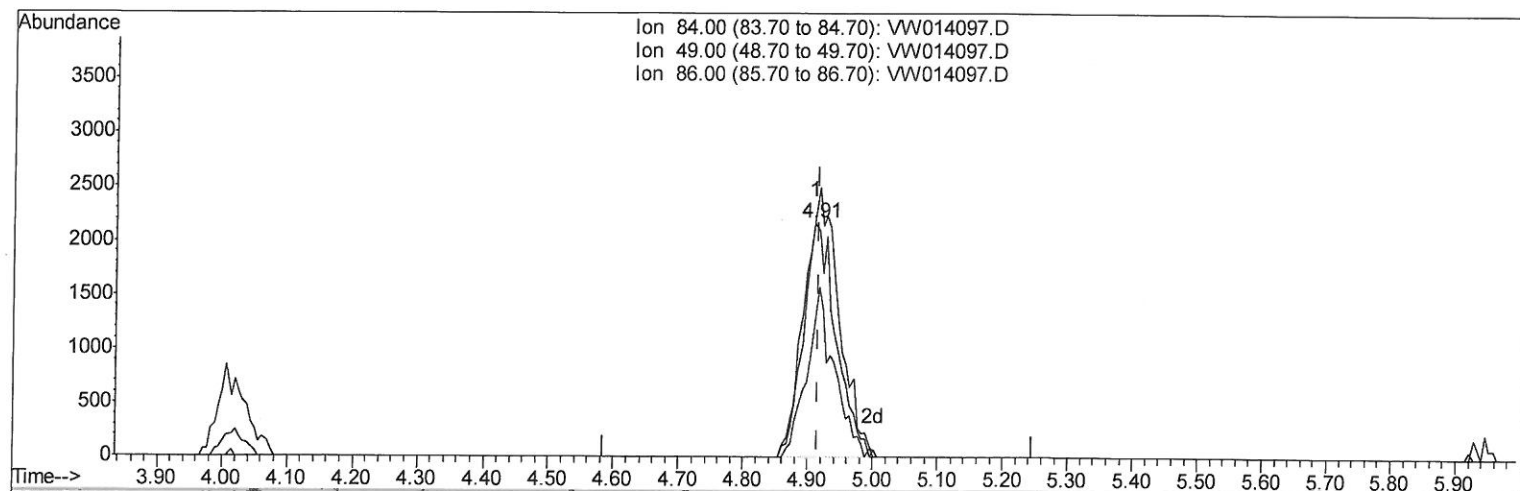

TIC: VW014097.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.62ug/L m

response 7585

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	100.46
86.00	62.40	55.61
0.00	0.00	0.00

> 11/25/19 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW112219\
Quantitation Report (QT Reviewed)

Data File : VW014097.D
Acq On : 22 Nov 2019 16:06
Operator : SY/VA
Sample : K5989-07
Misc : 4.90G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BK3

Manual Integrations
APPROVED

MMDadoda
11/26/2019 1:35:38 AM

Quant Time: Nov 22 23:44:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 22 23:01:18 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	243342	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	186932	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	56603	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	60850	15.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.68%
7) Chloroethane-d5	2.89	69	59703	18.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.88%
10) 1,1-Dichloroethene-d2	4.02	63	98651	12.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.52%
20) 2-Butanone-d5	7.07	46	58326	51.71	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.42%
24) Chloroform-d	7.65	84	165505	22.12	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.48%
26) 1,2-Dichloroethane-d4	8.31	65	91068	24.21	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.84%
29) Benzene-d6	8.27	84	327209	24.67	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.68%
33) 1,2-Dichloropropane-d6	9.27	67	106501	27.41	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.64%
37) Toluene-d8	10.32	98	260295	20.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.80%
38) trans-1,3-Dichloropropene-	10.58	79	29879	17.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.84%
39) 2-Hexanone-d5	10.92	63	41299	56.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.10%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	88233	30.07	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	120.28%#
61) 1,2-Dichlorobenzene-d4	13.85	152	55691	24.49	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.96%

Target Compounds

16) Methylene chloride	4.91	84	7585m	1.619	ug/L	Qvalue
------------------------	------	----	-------	-------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW112219\
Quantitation Report (QT Reviewed)

Data File : VW014097.D
Acq On : 22 Nov 2019 16:06
Operator : SY/VA
Sample : K5989-07
Misc : 4.90G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BK3

Manual Integrations
APPROVED

MMDadoda
11/26/2019 1:35:38 AM

Quant Time: Nov 22 23:44:57 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 22 23:01:18 2019
Response via : Initial Calibration

