

Data File : VW014106.D
Acq On : 25 Nov 2019 12:35
Operator : SY/VA
Sample : K6007-14
Misc : 5.96G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BM0

Quant Time: Nov 26 07:48:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 26 07:45:45 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	366542	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	347685	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	187404	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	94897	16.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.92%
7) Chloroethane-d5	2.89	69	91004	19.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.76%
10) 1,1-Dichloroethene-d2	4.02	63	163365	13.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.44%
20) 2-Butanone-d5	7.07	46	61448	36.17	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.34%
24) Chloroform-d	7.64	84	245642	21.80	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.20%
26) 1,2-Dichloroethane-d4	8.46	65	72	0.01	ug/L	0.16
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.04%#
29) Benzene-d6	8.27	84	519330	21.05	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.20%
33) 1,2-Dichloropropane-d6	9.27	67	155771	21.56	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.24%
37) Toluene-d8	10.32	98	478449	20.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.80%
38) trans-1,3-Dichloropropene-	10.57	79	57785	18.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.68%
39) 2-Hexanone-d5	10.92	63	45702	33.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.70%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	103852	19.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.12%
61) 1,2-Dichlorobenzene-d4	13.85	152	167494	22.25	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.00%

Target Compounds


					Qvalue
13) Acetone	4.12	43	4338	2.509 ug/L	48
16) Methylene chloride	4.91	84	18408	2.609 ug/L	95
42) cis-1,3-Dichloropropene	10.03	75	3628	0.374 ug/L #	71
59) 1,2,3-Trichloropropane	13.55	75	19284	4.869 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014106.D
Acq On : 25 Nov 2019 12:35
Operator : SY/VA
Sample : K6007-14
Misc : 5.96G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
COBM0

Quant Time: Nov 26 07:48:11 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 26 07:45:45 2019
Response via : Initial Calibration

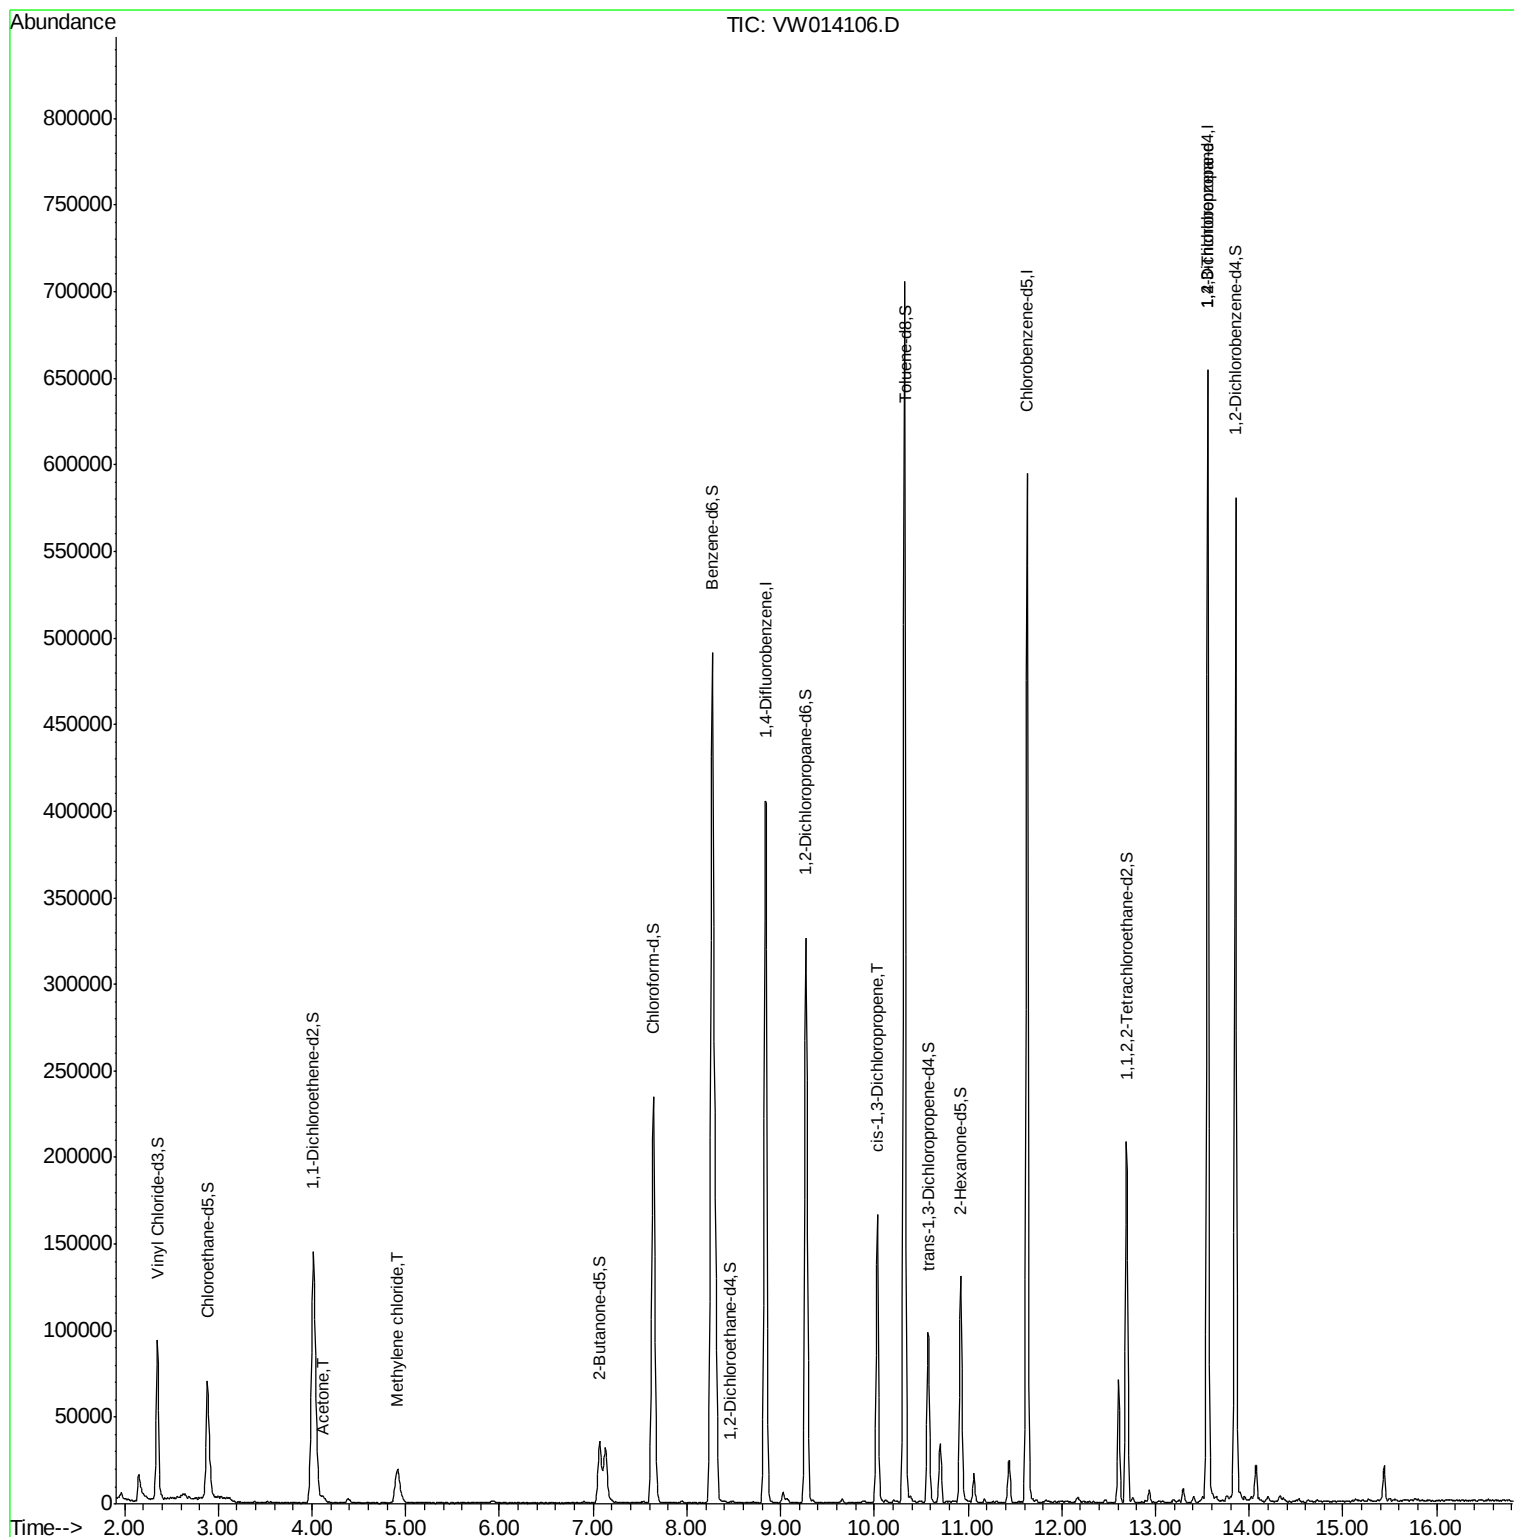

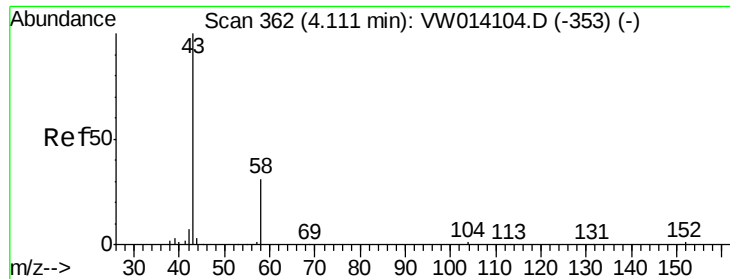

#13

Acetone

Concen: 2.509 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW014106.D

Acq: 25 Nov 2019 12:35

Instrument :

MSVOA_W

ClientSampleId :


COBMO

Tgt Ion: 43 Resp: 4338

Ion Ratio Lower Upper




43 100

58 3.7 0.0 65.4

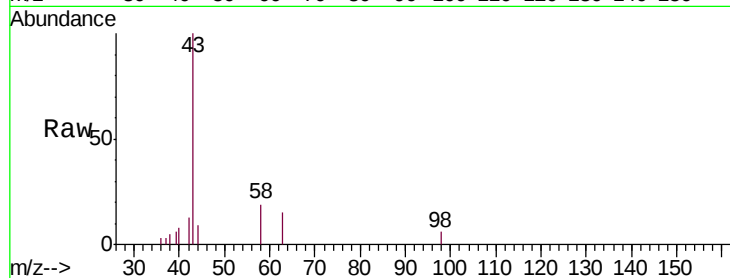

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

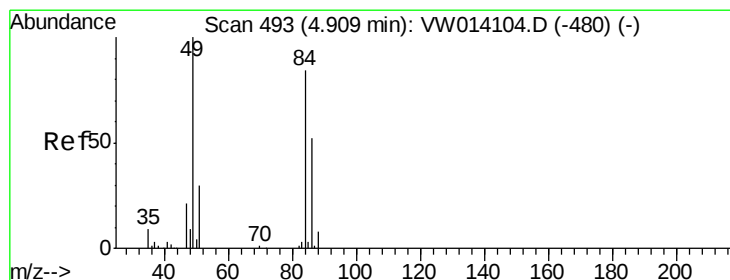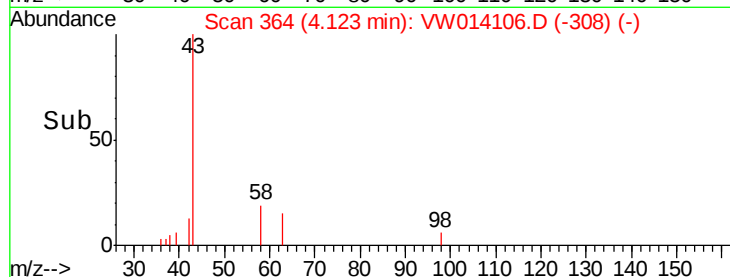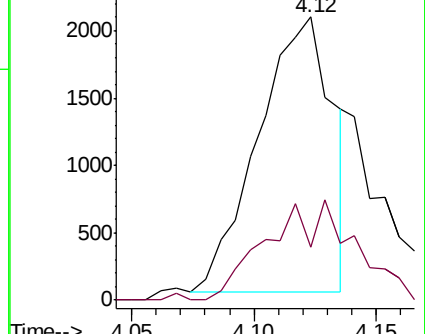

#16

Methylene chloride

Concen: 2.609 ug/L

RT: 4.91 min Scan# 493

Delta R.T. -0.00 min

Lab File: VW014106.D

Acq: 25 Nov 2019 12:35


Tgt Ion: 84 Resp: 18408

Ion Ratio Lower Upper

84 100

49 118.2 84.2 156.4



86 53.5 43.7 81.1

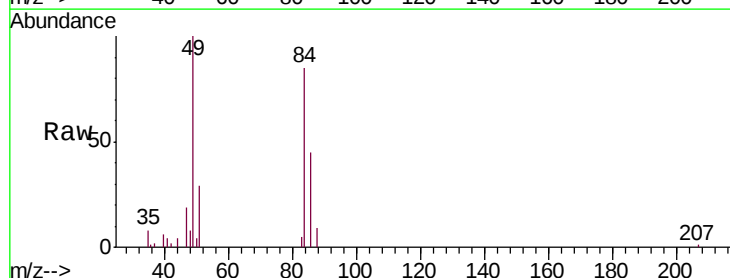


Abundance Ion 84.00 (83.70 to 84.70): VW

Ion 49.00 (48.70 to 49.70): VW

Ion 86.00 (85.70 to 86.70): VW

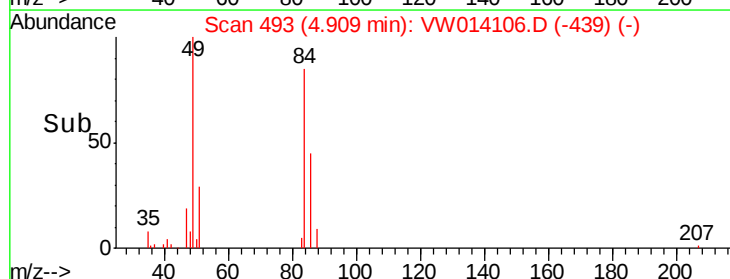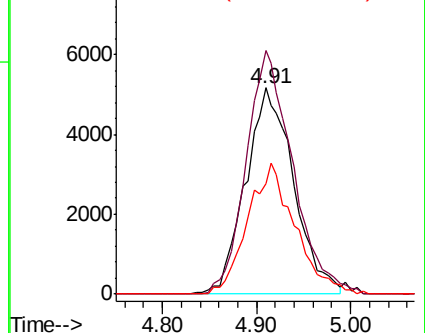

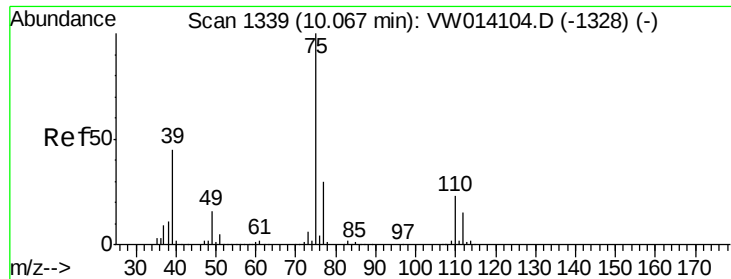

#42

cis-1,3-Dichloropropene

Concen: 0.374 ug/L

RT: 10.03 min Scan# 1333

Delta R.T. -0.04 min

Lab File: VW014106.D

Acq: 25 Nov 2019 12:35

Instrument :

MSVOA_W

ClientSampleId :





COBMO

Tgt Ion: 75 Resp: 3628

Ion Ratio Lower Upper

75 100

77 47.5 22.1 41.1#

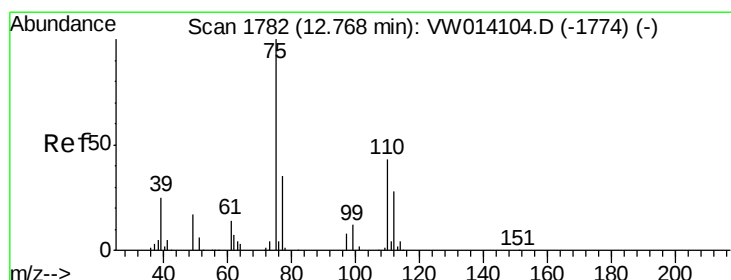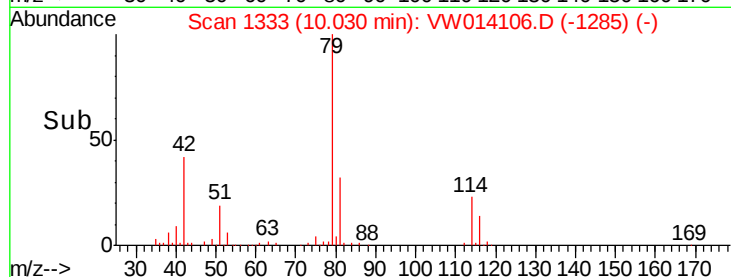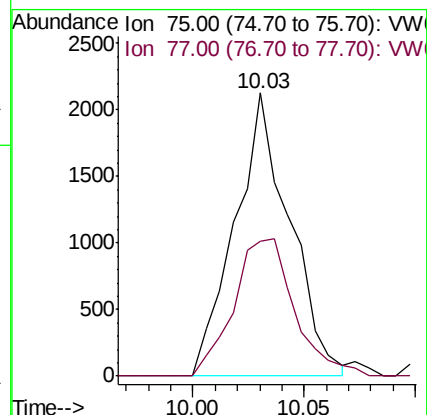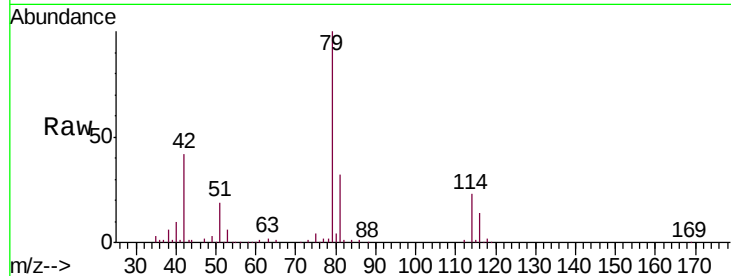

#59

1,2,3-Trichloropropane

Concen: 4.869 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW014106.D

Acq: 25 Nov 2019 12:35

Tgt Ion: 75 Resp: 19284

Ion Ratio Lower Upper

75 100

77 34.8 25.9 38.9

