

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112519\
 Data File : VW014117.D
 Acq On : 25 Nov 2019 17:47
 Operator : SY/VA
 Sample : K6007-16
 Misc : 3.20G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BM2

Quant Time: Nov 26 07:49:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 26 07:45:45 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 11/27/2019 5:13:32 PM

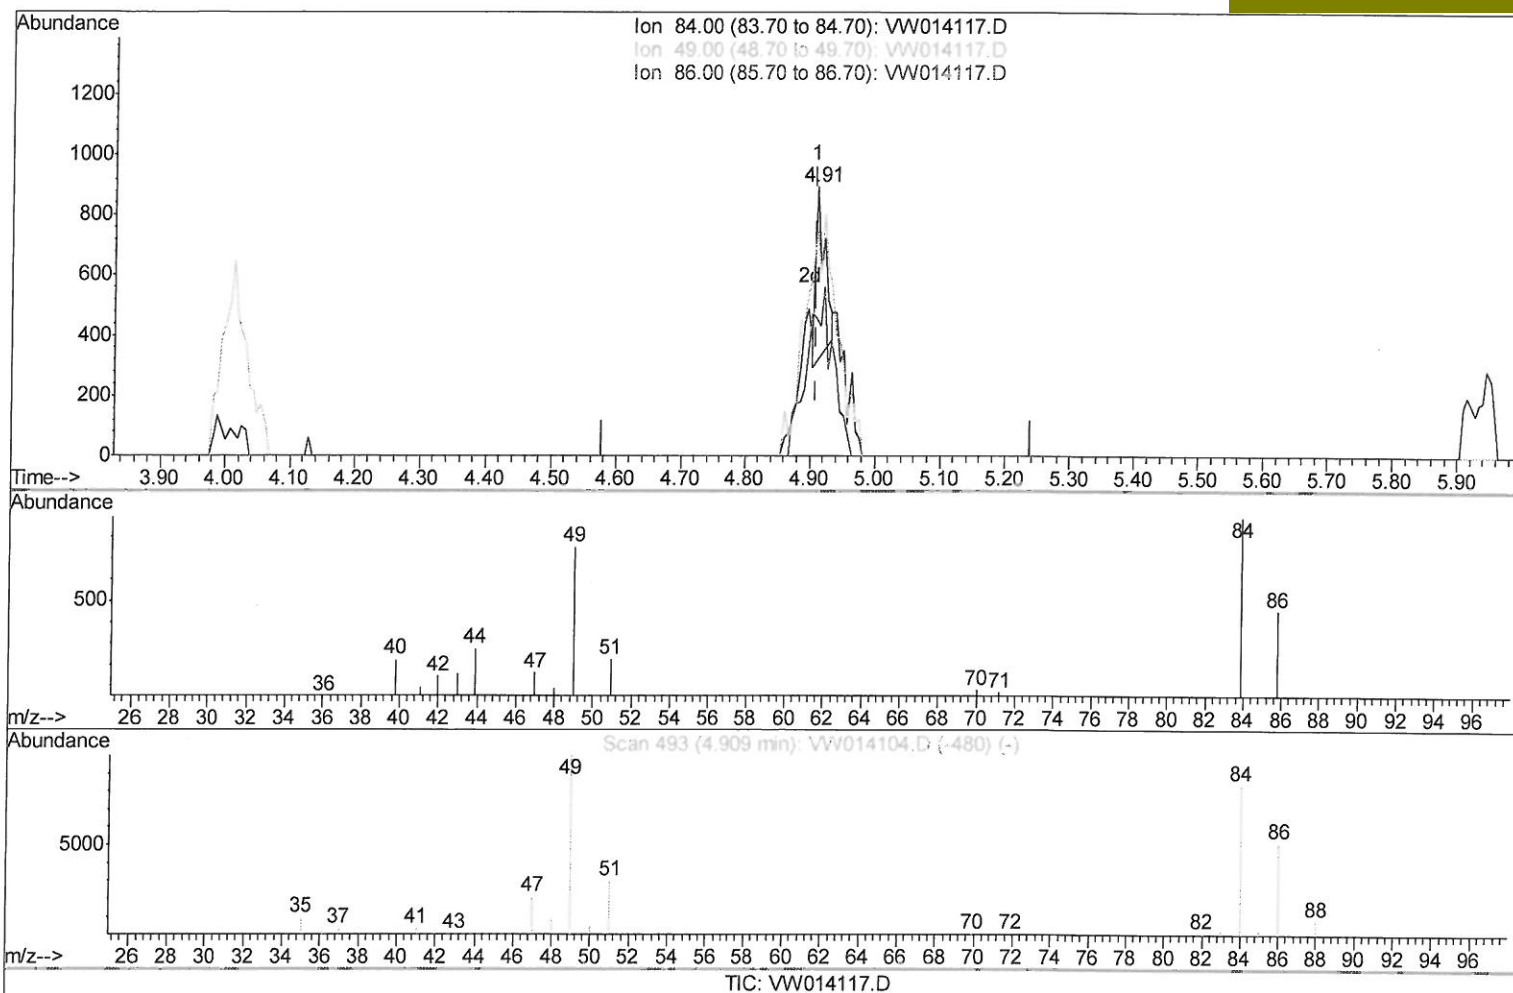

(16) Methylene chloride (T)

4.909min (-0.000) 0.37ug/L

response 557

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	84.23
86.00	62.40	51.01
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112519\
 Data File : VW014117.D
 Acq On : 25 Nov 2019 17:47
 Operator : SY/VA
 Sample : K6007-16
 Misc : 3.20G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 C0BM2

Quant Time: Nov 26 07:49:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 26 07:45:45 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 11/27/2019 5:13:32 PM

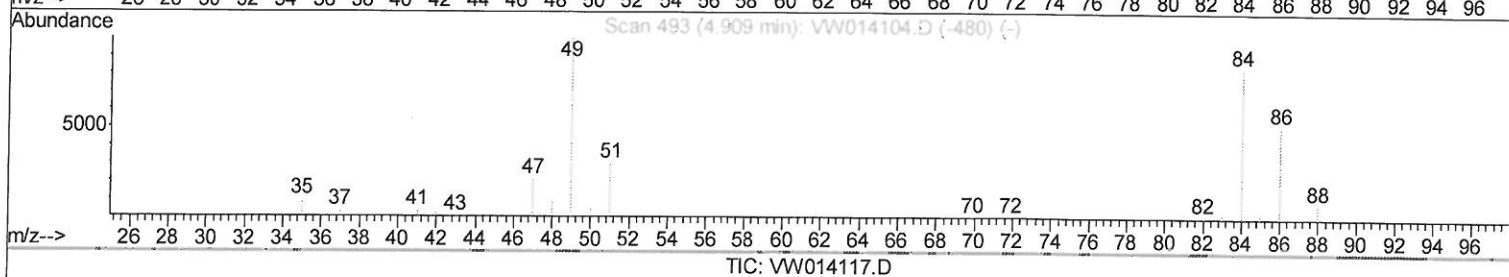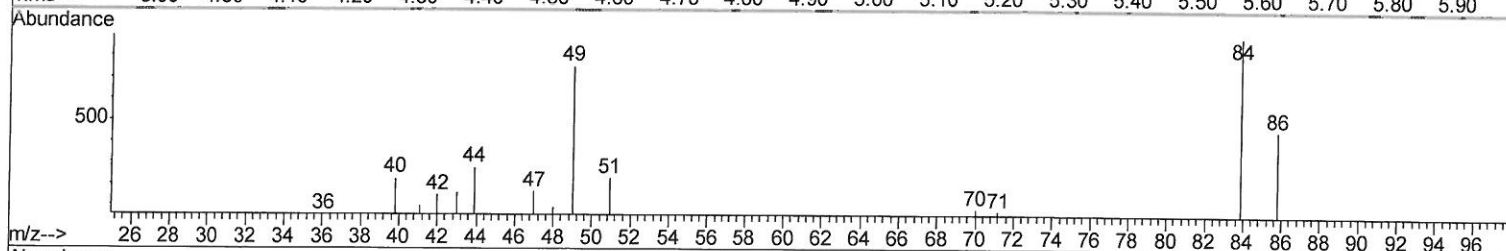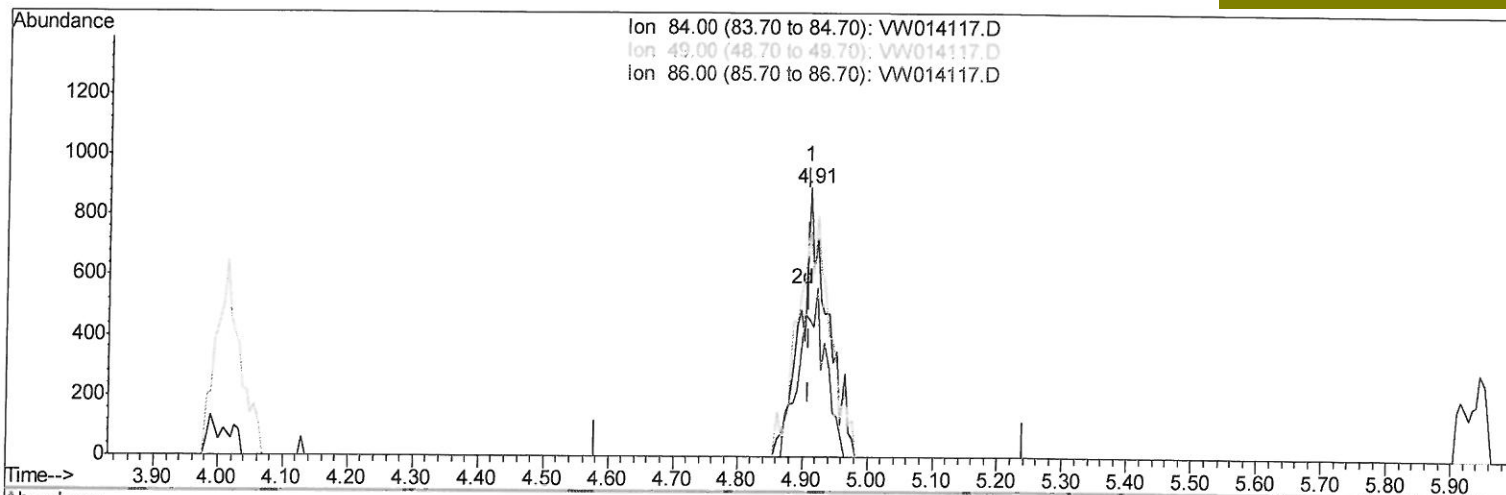

TIC: VW014117.D

(16) Methylene chloride (T)

4.909min (-0.000) 1.67ug/L m

511/29/19 Sy

response 2534

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	84.23
86.00	62.40	51.01
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112519\
 Data File : VW014117.D
 Acq On : 25 Nov 2019 17:47
 Operator : SY/VA
 Sample : K6007-16
 Misc : 3.20G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 C0BM2

Quant Time: Nov 26 07:49:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 26 07:45:45 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 11/27/2019 5:13:32 PM

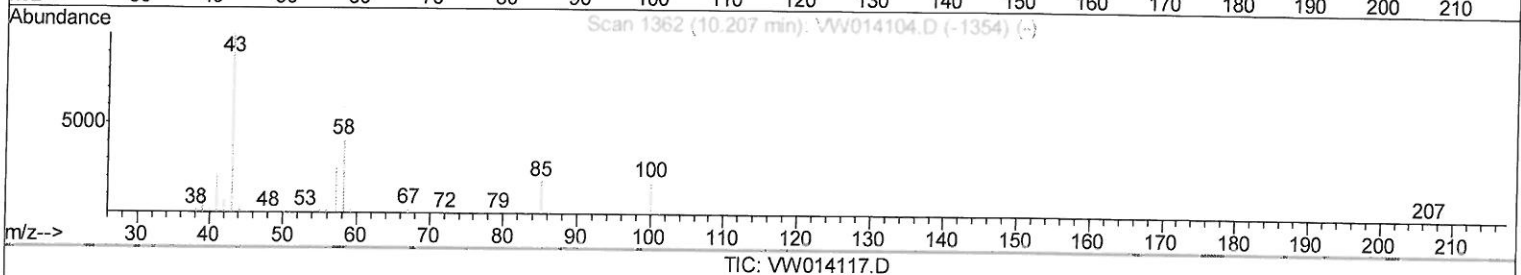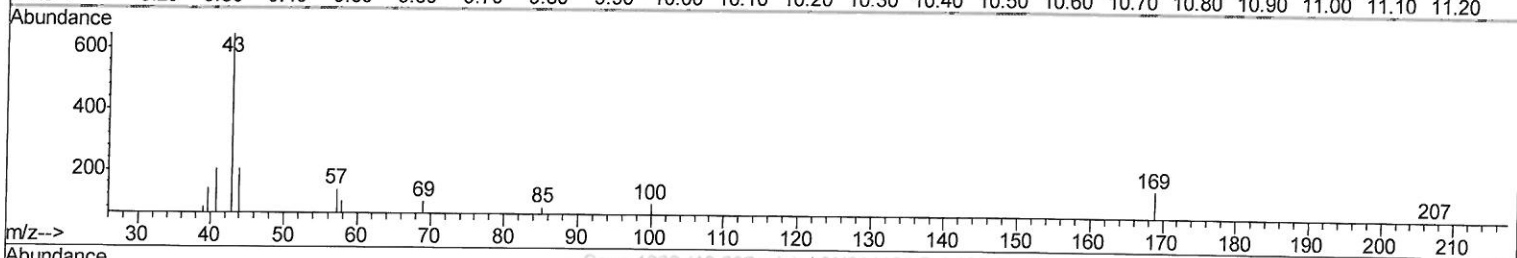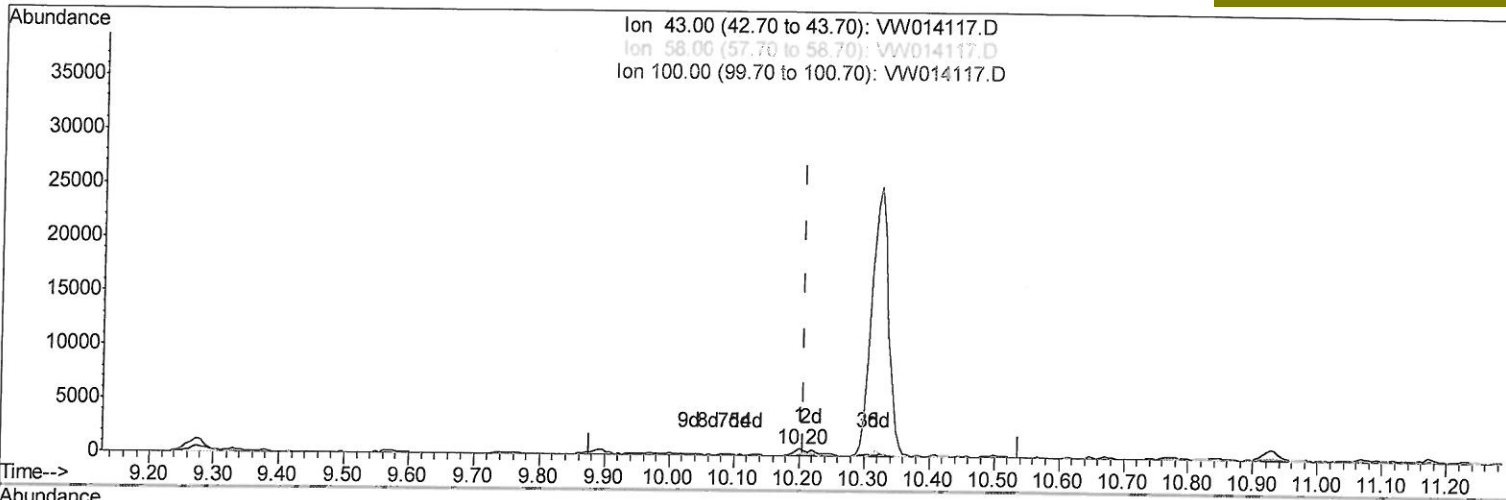

(43) 4-Methyl-2-pentanone (T)

10.201min (-0.006) 2.88ug/L

response 844

Ion	Exp%	Act%
43.00	100	100
58.00	40.80	39.10
100.00	17.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112519\
 Data File : VW014117.D
 Acq On : 25 Nov 2019 17:47
 Operator : SY/VA
 Sample : K6007-16
 Misc : 3.20G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BM2

Quant Time: Nov 26 07:49:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 26 07:45:45 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 11/27/2019 5:13:32 PM

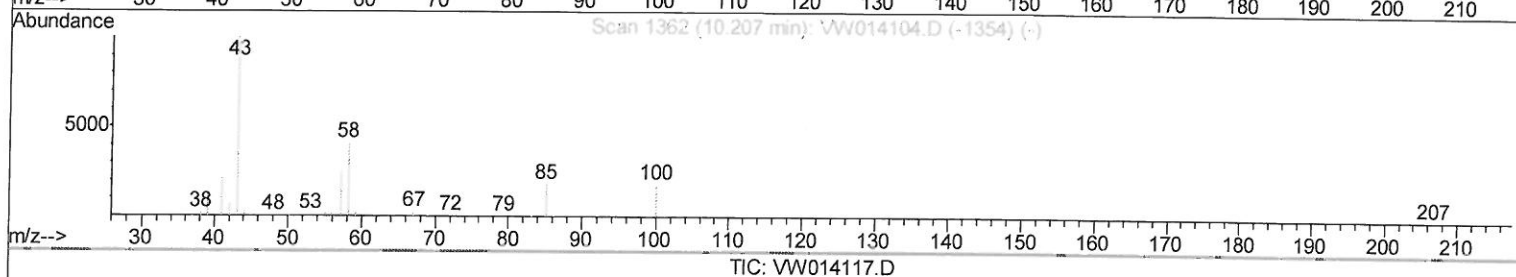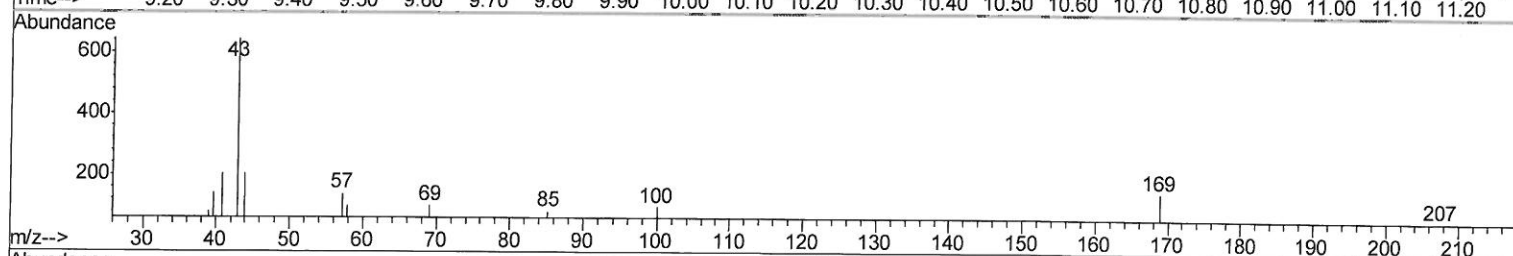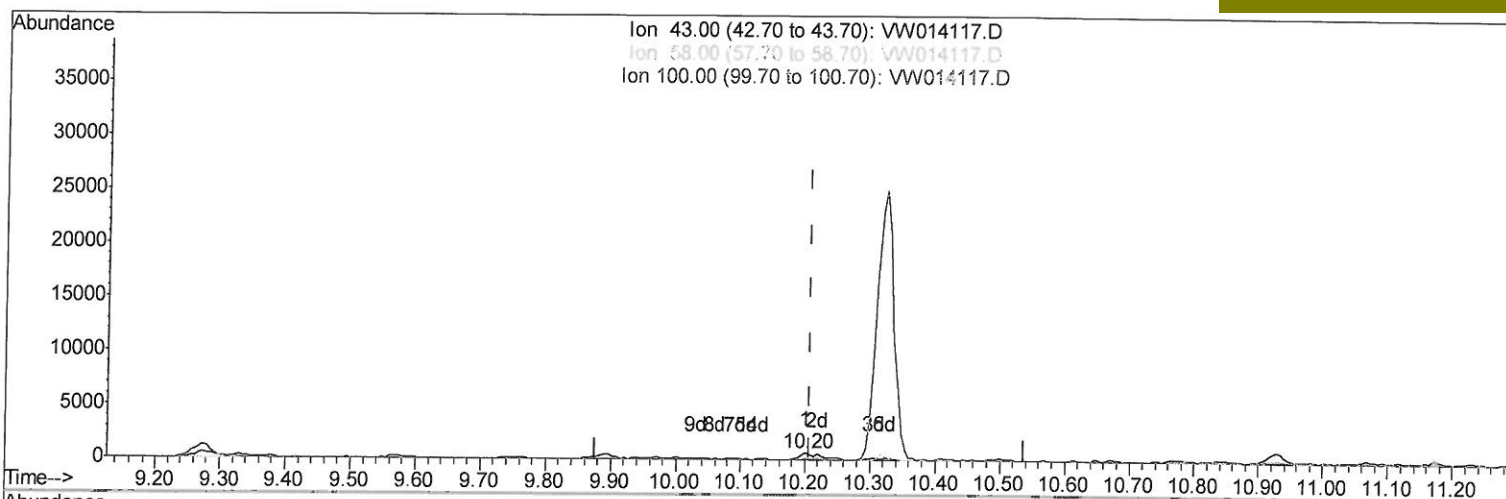

(43) 4-Methyl-2-pentanone (T)

10.201min (-0.006) 5.05ug/L m) 11/29/19 SY

response 1478

Ion	Exp%	Act%
43.00	100	100
58.00	40.80	22.33#
100.00	17.30	0.00#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112519\
 Data File : VW014117.D
 Acq On : 25 Nov 2019 17:47
 Operator : SY/VA
 Sample : K6007-16
 Misc : 3.20G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 COBM2

Quant Time: Nov 26 08:40:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 26 07:45:45 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 11/27/2019 5:13:32 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	78632	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	25110	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	2900	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	52500	41.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	167.40%#
7) Chloroethane-d5	2.89	69	55662	54.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	218.92%#
10) 1,1-Dichloroethene-d2	4.01	63	66702	25.91	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	103.64%#
20) 2-Butanone-d5	7.07	46	56991	156.37	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	312.74%#
24) Chloroform-d	7.64	84	126217	52.20	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	208.80%#
26) 1,2-Dichloroethane-d4	8.30	65	46264	38.06	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	152.24%#
29) Benzene-d6	8.27	84	202339	113.57	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	454.28%#
33) 1,2-Dichloropropane-d6	9.27	67	63804	122.26	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	489.04%#
37) Toluene-d8	10.32	98	67555	39.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	159.92%#
38) trans-1,3-Dichloropropene-	10.58	79	5228	23.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.56%#
39) 2-Hexanone-d5	10.93	63	10252	103.59	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	207.18%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	26920	68.31	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	273.24%#
61) 1,2-Dichlorobenzene-d4	13.85	152	4048	34.74	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	138.96%#

Target Compounds

					Qvalue	
13) Acetone	4.12	43	8408	22.671	ug/L	86
16) Methylene chloride	4.91	84	2534m	1.674	ug/L	
19) 1,1-Dichloroethane	6.21	63	1369	0.587	ug/L #	84
30) Cyclohexane	7.95	56	2562	3.188	ug/L #	88
31) 1,1,1-Trichloroethane	7.87	97	52037	82.693	ug/L	99
36) Methylcyclohexane	9.33	83	6345	7.203	ug/L	95
43) 4-Methyl-2-pentanone	10.20	43	1478m	5.049	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112519\
Data File : VW014117.D
Acq On : 25 Nov 2019 17:47
Operator : SY/VA
Sample : K6007-16
Misc : 3.20G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0BM2

Quant Time: Nov 26 08:40:03 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 26 07:45:45 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

apatel
11/27/2019 5:13:32 PM

