

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW112519\
 Data File : VW014120.D
 Acq On : 25 Nov 2019 19:07
 Operator : SY/VA
 Sample : K6007-19
 Misc : 6.12G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BM5

Quant Time: Nov 26 08:53:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 26 07:45:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	231737	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	229988	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	125416	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	58820	15.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.64%
7) Chloroethane-d5	2.89	69	58897	19.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.60%
10) 1,1-Dichloroethene-d2	4.01	63	104556	13.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.12%
20) 2-Butanone-d5	7.07	46	62564	58.25	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.50%
24) Chloroform-d	7.65	84	166172	23.32	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.28%
26) 1,2-Dichloroethane-d4	8.31	65	95638	26.70	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.80%
29) Benzene-d6	8.27	84	335942	20.59	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.36%
33) 1,2-Dichloropropane-d6	9.27	67	106812	22.35	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.40%
37) Toluene-d8	10.32	98	307193	19.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.40%
38) trans-1,3-Dichloropropene-	10.57	79	44163	21.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.28%
39) 2-Hexanone-d5	10.92	63	47268	52.15	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.30%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	98818	27.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	115702	22.96	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.84%


Target Compounds					Ovalue
13) Acetone	4.12	43	4363	3.992 ug/L	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW112519\
Data File : VW014120.D
Acq On : 25 Nov 2019 19:07
Operator : SY/VA
Sample : K6007-19
Misc : 6.12G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BM5

Quant Time: Nov 26 08:53:06 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 26 07:45:45 2019
Response via : Initial Calibration

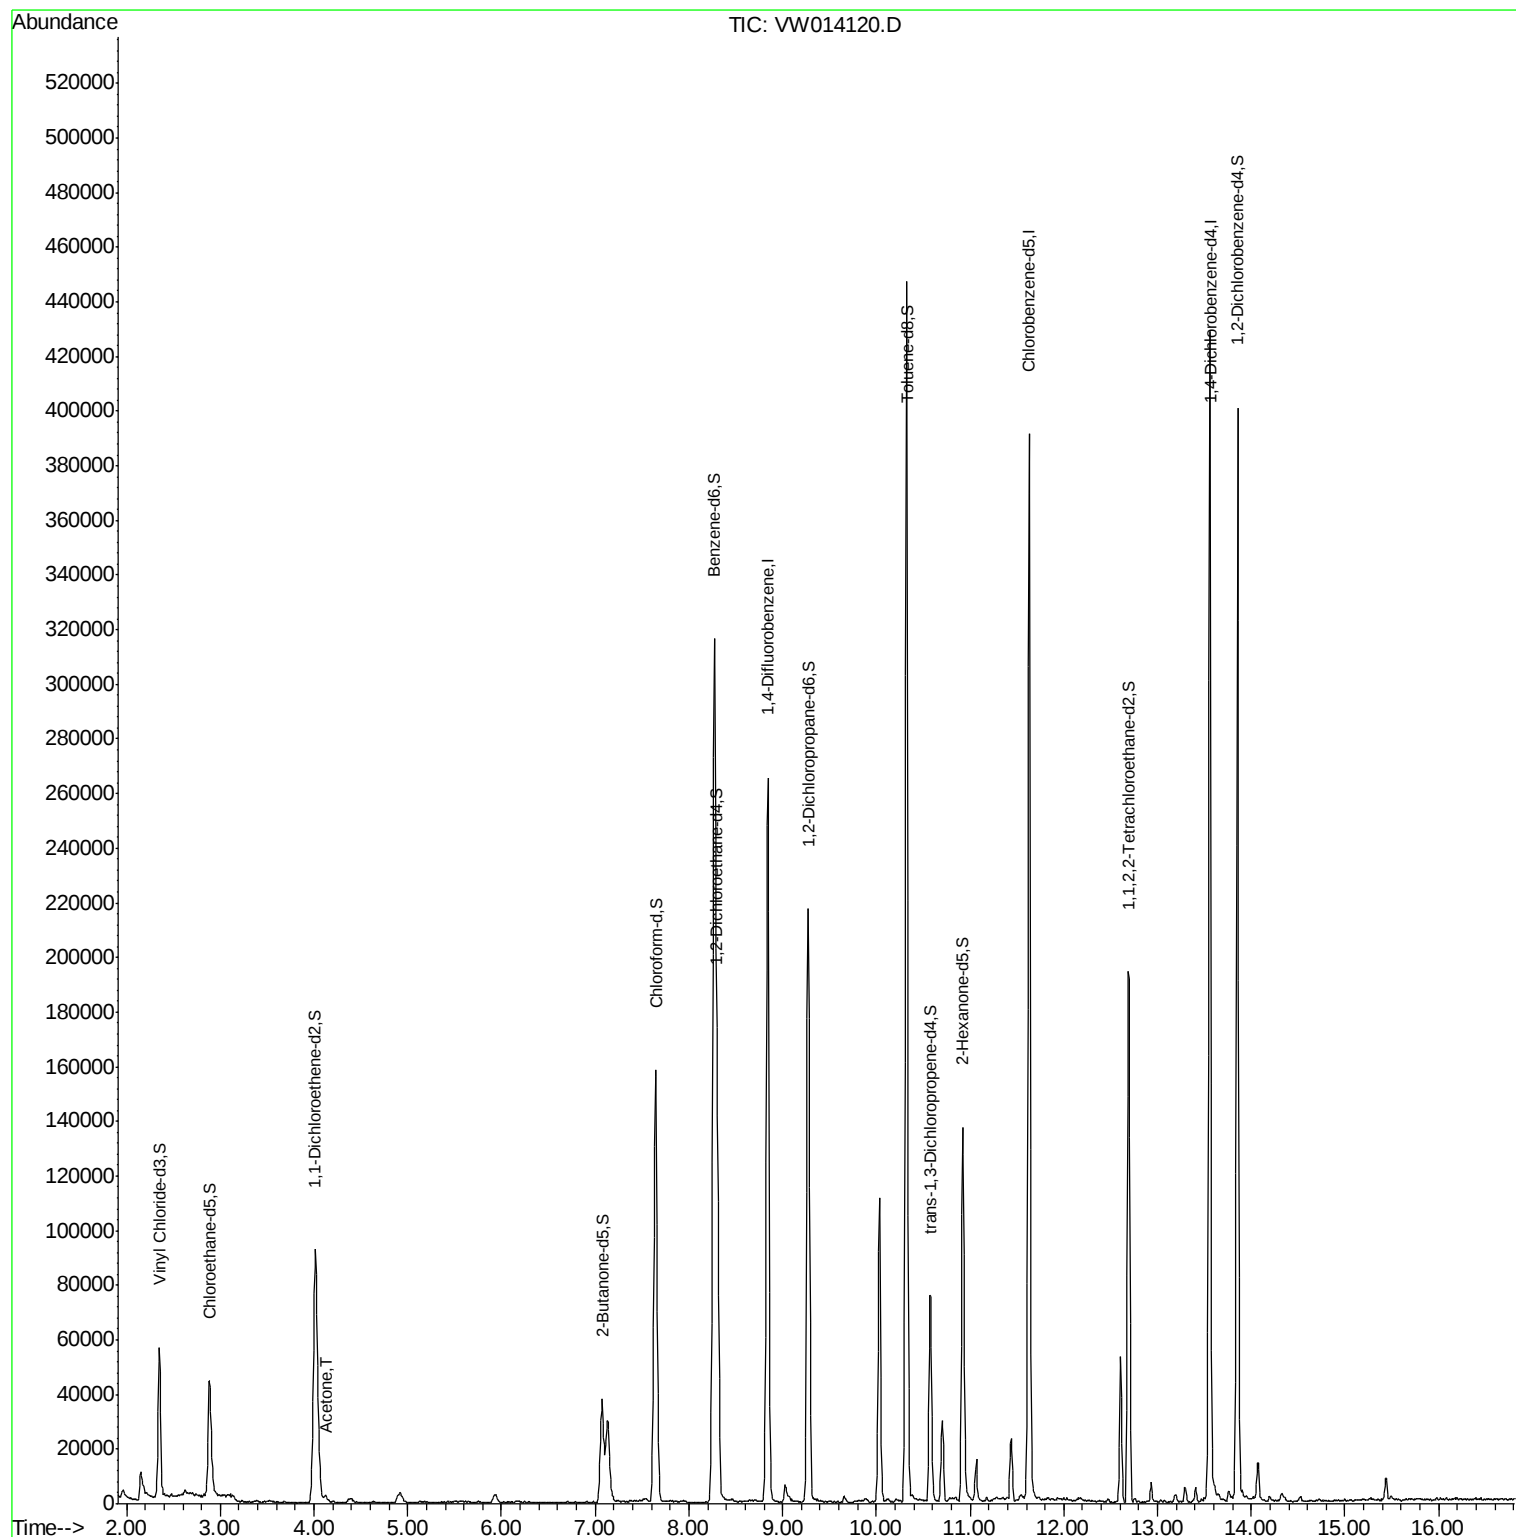

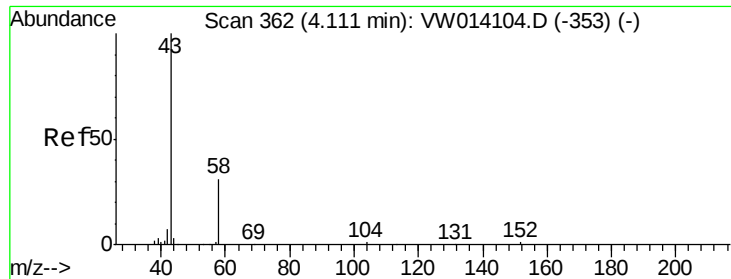

#13

Acetone

Concen: 3.992 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW014120.D

Acq: 25 Nov 2019 19:07

Instrument :
MSVOA_W
ClientSampleId :
C0BM5

Tot Ion: 43 Resp: 4363

Ion Ratio Lower Upper

43 100

58 12.6 0.0 65.4

