
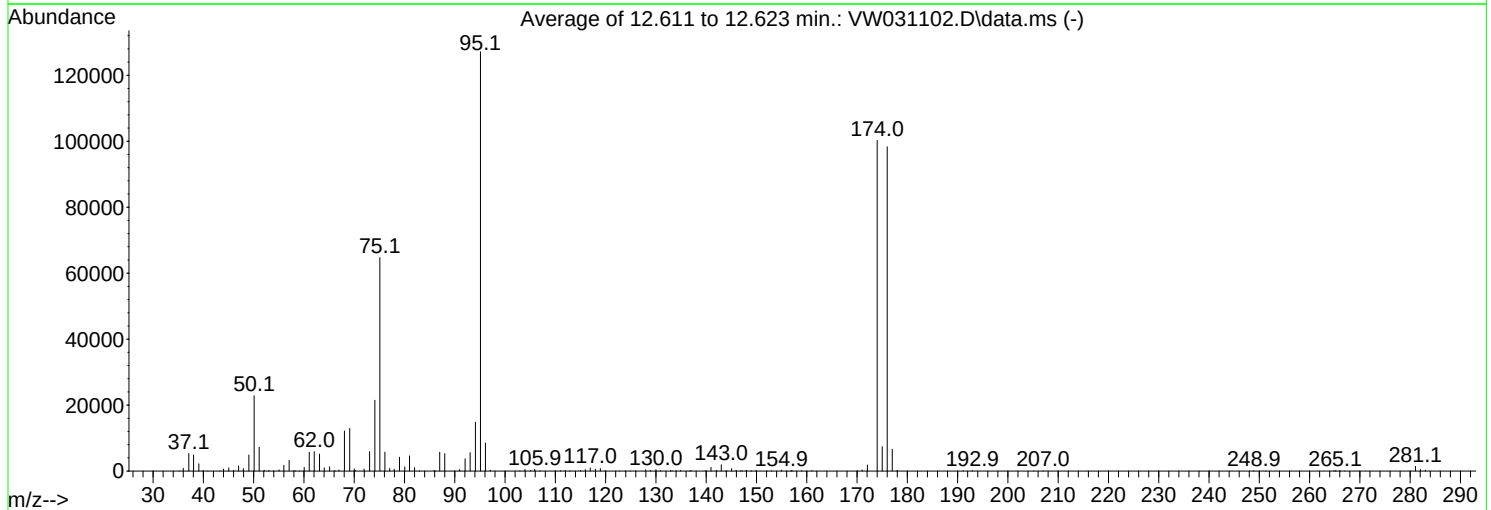


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112524\
Data File : VW031102.D
Acq On : 25 Nov 2024 08:41
Operator : SY/MD
Sample : BFB405
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB405

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM112024SMA.M
Title : SFAM01.0
Last Update : Tue Nov 26 05:01:26 2024

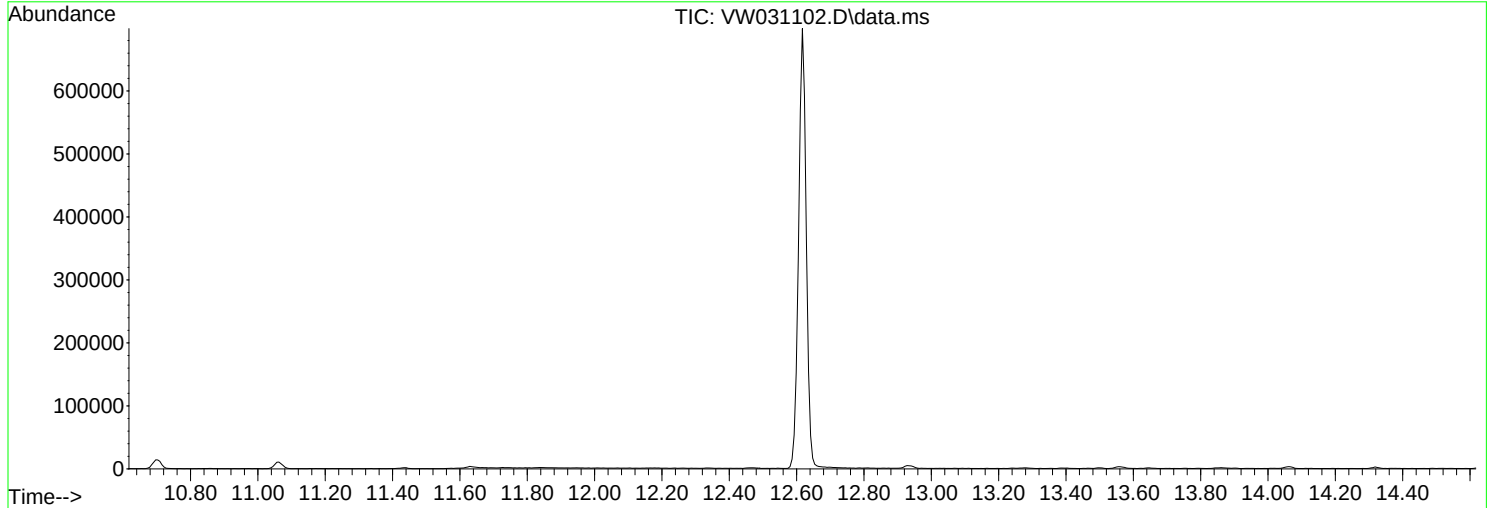

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	22851	PASS
75	95	30	80	50.9	64723	PASS
95	95	100	100	100.0	127147	PASS
96	95	5	9	6.7	8536	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.9	100256	PASS
175	174	5	9	7.4	7413	PASS
176	174	95	101	98.1	98336	PASS
177	176	5	9	6.7	6625	PASS

m/z	Abundance
36.00	367.0
38.00	113.0
39.90	185.0
44.00	152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB405

m/z	Abundance
36.00	1196.0
37.10	5382.0
38.10	4994.0
39.10	2270.0
40.00	282.0
44.00	761.0
45.10	1100.0
45.90	309.0
47.00	1181.0
47.90	765.0
49.00	4636.0
50.10	22184.0
51.10	6868.0
52.10	297.0
52.90	181.0
54.00	128.0
55.10	333.0
56.00	1723.0
57.10	3071.0
58.30	156.0
59.10	69.0
60.00	1065.0
61.00	5819.0
62.00	5793.0
63.10	5339.0
64.10	1190.0
65.10	1428.0
66.20	287.0
67.00	354.0
68.10	11846.0
69.10	12498.0
70.00	1033.0
72.00	622.0
73.10	6047.0
74.10	21496.0
75.10	62192.0
76.10	5467.0
77.10	724.0
78.00	640.0
79.00	4025.0
80.00	1233.0
81.00	4870.0
82.00	960.0
83.10	84.0
85.90	209.0
87.00	5479.0
88.00	4541.0
91.00	468.0
92.00	3742.0
93.00	4811.0
94.10	13662.0
95.10	118424.0
96.10	7739.0
97.20	213.0
103.90	387.0
105.10	197.0
105.90	513.0
107.00	74.0
110.10	84.0
111.00	137.0
112.00	76.0
112.90	60.0
114.90	198.0
115.90	484.0
117.00	1059.0
117.90	473.0
119.00	633.0
122.80	62.0
124.90	124.0
126.00	69.0
128.00	292.0
129.00	219.0
130.00	460.0
131.00	122.0
132.90	214.0
133.20	190.0
134.00	161.0
134.90	205.0
136.70	134.0
137.00	127.0
139.90	93.0
141.00	967.0
142.10	87.0
143.00	2030.0
144.10	96.0
145.10	894.0
145.90	203.0
146.90	129.0
147.90	264.0
149.10	105.0
149.90	95.0
153.00	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB405

155.10	254.0
156.70	111.0
157.20	139.0
158.90	122.0
161.10	134.0
171.00	306.0
172.10	2166.0
174.00	84096.0
175.00	6315.0
176.00	80960.0
177.00	5779.0
177.90	211.0
191.20	172.0
193.00	256.0
205.20	66.0
207.00	175.0
248.90	170.0
251.30	106.0
265.10	411.0
266.00	100.0
267.00	99.0
281.10	2480.0
282.10	728.0
283.00	365.0

Instrument :
MSVOA_W
ClientSampleId :
BFB405

m/z	Abundance
36.10	1427.0
37.10	5892.0
38.10	5653.0
39.10	2412.0
39.90	343.0
43.30	57.0
44.10	924.0
45.00	1024.0
46.00	207.0
47.00	2142.0
47.90	769.0
49.00	5481.0
50.10	26312.0
51.10	8674.0
52.10	289.0
53.10	130.0
53.90	77.0
55.10	434.0
56.00	1848.0
57.00	3506.0
58.00	189.0
60.10	1360.0
61.10	6243.0
62.10	6829.0
63.10	6168.0
64.00	1083.0
65.10	1449.0
66.00	104.0
66.90	415.0
68.00	13633.0
69.10	14765.0
70.00	968.0
72.00	691.0
73.00	6264.0
74.10	24008.0
75.10	74512.0
76.10	6596.0
77.10	886.0
77.90	637.0
79.00	4801.0
80.10	1431.0
81.00	5312.0
82.00	1099.0
83.00	78.0
86.10	196.0
87.00	6836.0
88.00	6171.0
91.00	482.0
92.10	3882.0
93.10	6348.0
94.10	17120.0
95.10	144000.0
96.10	9851.0
97.00	333.0
103.00	71.0
103.90	518.0
105.00	194.0
105.90	594.0
106.90	171.0
109.90	84.0
111.00	173.0
111.90	93.0
112.90	108.0
115.00	212.0
116.00	477.0
117.00	966.0
118.00	732.0
118.90	967.0
119.90	77.0
123.90	61.0
124.90	72.0
126.00	110.0
127.90	447.0
128.90	200.0
130.10	477.0
130.80	191.0
132.90	178.0
134.00	82.0
134.90	234.0
136.90	205.0
139.90	154.0
140.90	1281.0
142.00	240.0
143.00	1872.0
144.10	93.0
145.00	857.0
146.00	235.0
146.80	110.0
147.20	97.0
148.00	325.0
148.90	145.0
149.90	152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB405

152.10	95.0
152.90	82.0
154.90	438.0
156.10	55.0
156.90	245.0
158.90	168.0
161.00	129.0
171.00	376.0
172.10	1928.0
174.00	111800.0
175.00	8121.0
176.00	109216.0
177.00	7434.0
178.00	205.0
191.00	148.0
192.90	150.0
205.10	79.0
207.00	99.0
248.90	174.0
264.80	169.0
265.30	129.0
266.20	67.0
281.00	1283.0
282.00	484.0
283.10	307.0

Instrument :
MSVOA_W
ClientSampleId :
BFB405

m/z	Abundance
35.20	79.0
36.10	1043.0
37.10	4721.0
38.10	4357.0
39.10	1981.0
40.00	263.0
40.90	63.0
44.10	551.0
45.10	820.0
46.10	169.0
47.00	1343.0
48.00	698.0
49.10	4501.0
50.10	20056.0
51.10	6177.0
52.10	252.0
53.00	117.0
53.90	56.0
55.00	340.0
56.00	1706.0
57.10	3187.0
58.00	117.0
60.00	973.0
61.00	5114.0
62.00	5017.0
63.10	3948.0
64.10	642.0
65.10	1037.0
66.10	192.0
67.00	268.0
68.10	10938.0
69.10	11582.0
70.20	666.0
71.90	599.0
73.00	5472.0
74.10	18904.0
75.10	57464.0
76.10	5147.0
77.00	798.0
78.00	482.0
79.00	3816.0
80.00	1106.0
81.00	3670.0
82.00	1066.0
83.00	172.0
85.90	187.0
87.00	4849.0
88.00	5221.0
90.90	462.0
92.00	3580.0
93.00	5654.0
94.10	13676.0
95.10	119016.0
96.10	8017.0
97.00	316.0
102.90	172.0
104.00	648.0
105.00	123.0
105.90	535.0
107.00	116.0
109.90	52.0
111.00	110.0
111.90	66.0
112.90	72.0
115.10	105.0
115.90	389.0
116.90	844.0
118.00	509.0
119.00	719.0
123.90	116.0
128.00	442.0
128.80	208.0
129.90	387.0
130.90	125.0
132.80	96.0
134.90	164.0
137.00	253.0
139.90	123.0
141.00	1198.0
142.20	240.0
143.00	1882.0
143.80	156.0
145.00	538.0
145.90	207.0
146.80	93.0
147.10	89.0
147.90	236.0
148.80	97.0
149.90	87.0
152.10	71.0
152.90	102.0
155.00	278.0

Instrument :
MSVOA_W
ClientSampleId :
BFB405

156.00	74.0
157.00	275.0
159.00	136.0
160.90	112.0
170.00	76.0
171.00	368.0
172.00	1419.0
174.00	104872.0
175.00	7803.0
176.00	104832.0
177.00	6662.0
178.00	280.0
192.80	64.0
265.20	70.0
281.20	621.0
282.20	193.0
283.00	138.0

Instrument :
MSVOA_W
ClientSampleId :
BFB405