

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112625\
 Data File : VW032552.D
 Acq On : 26 Nov 2025 18:17
 Operator : SY/MD
 Sample : Q3719-13
 Misc : 5.39g/5mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-1125-17A

Quant Time: Nov 27 00:31:28 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111025S.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 11 03:48:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.959	168	171429	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.849	114	419256	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.635	117	506374	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.555	152	251247	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	165549	74.905	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	149.800%
35) Dibromofluoromethane	7.904	113	139819	55.701	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	111.400%
50) Toluene-d8	10.330	98	473523	49.172	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	98.340%
62) 4-Bromofluorobenzene	12.617	95	219295	60.282	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	120.560%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW112625\
Data File : VW032552.D
Acq On : 26 Nov 2025 18:17
Operator : SY/MD
Sample : Q3719-13
Misc : 5.39g/5mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-1125-17A

Quant Time: Nov 27 00:31:28 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111025S.M
Quant Title : SW846 8260
QLast Update : Tue Nov 11 03:48:21 2025
Response via : Initial Calibration




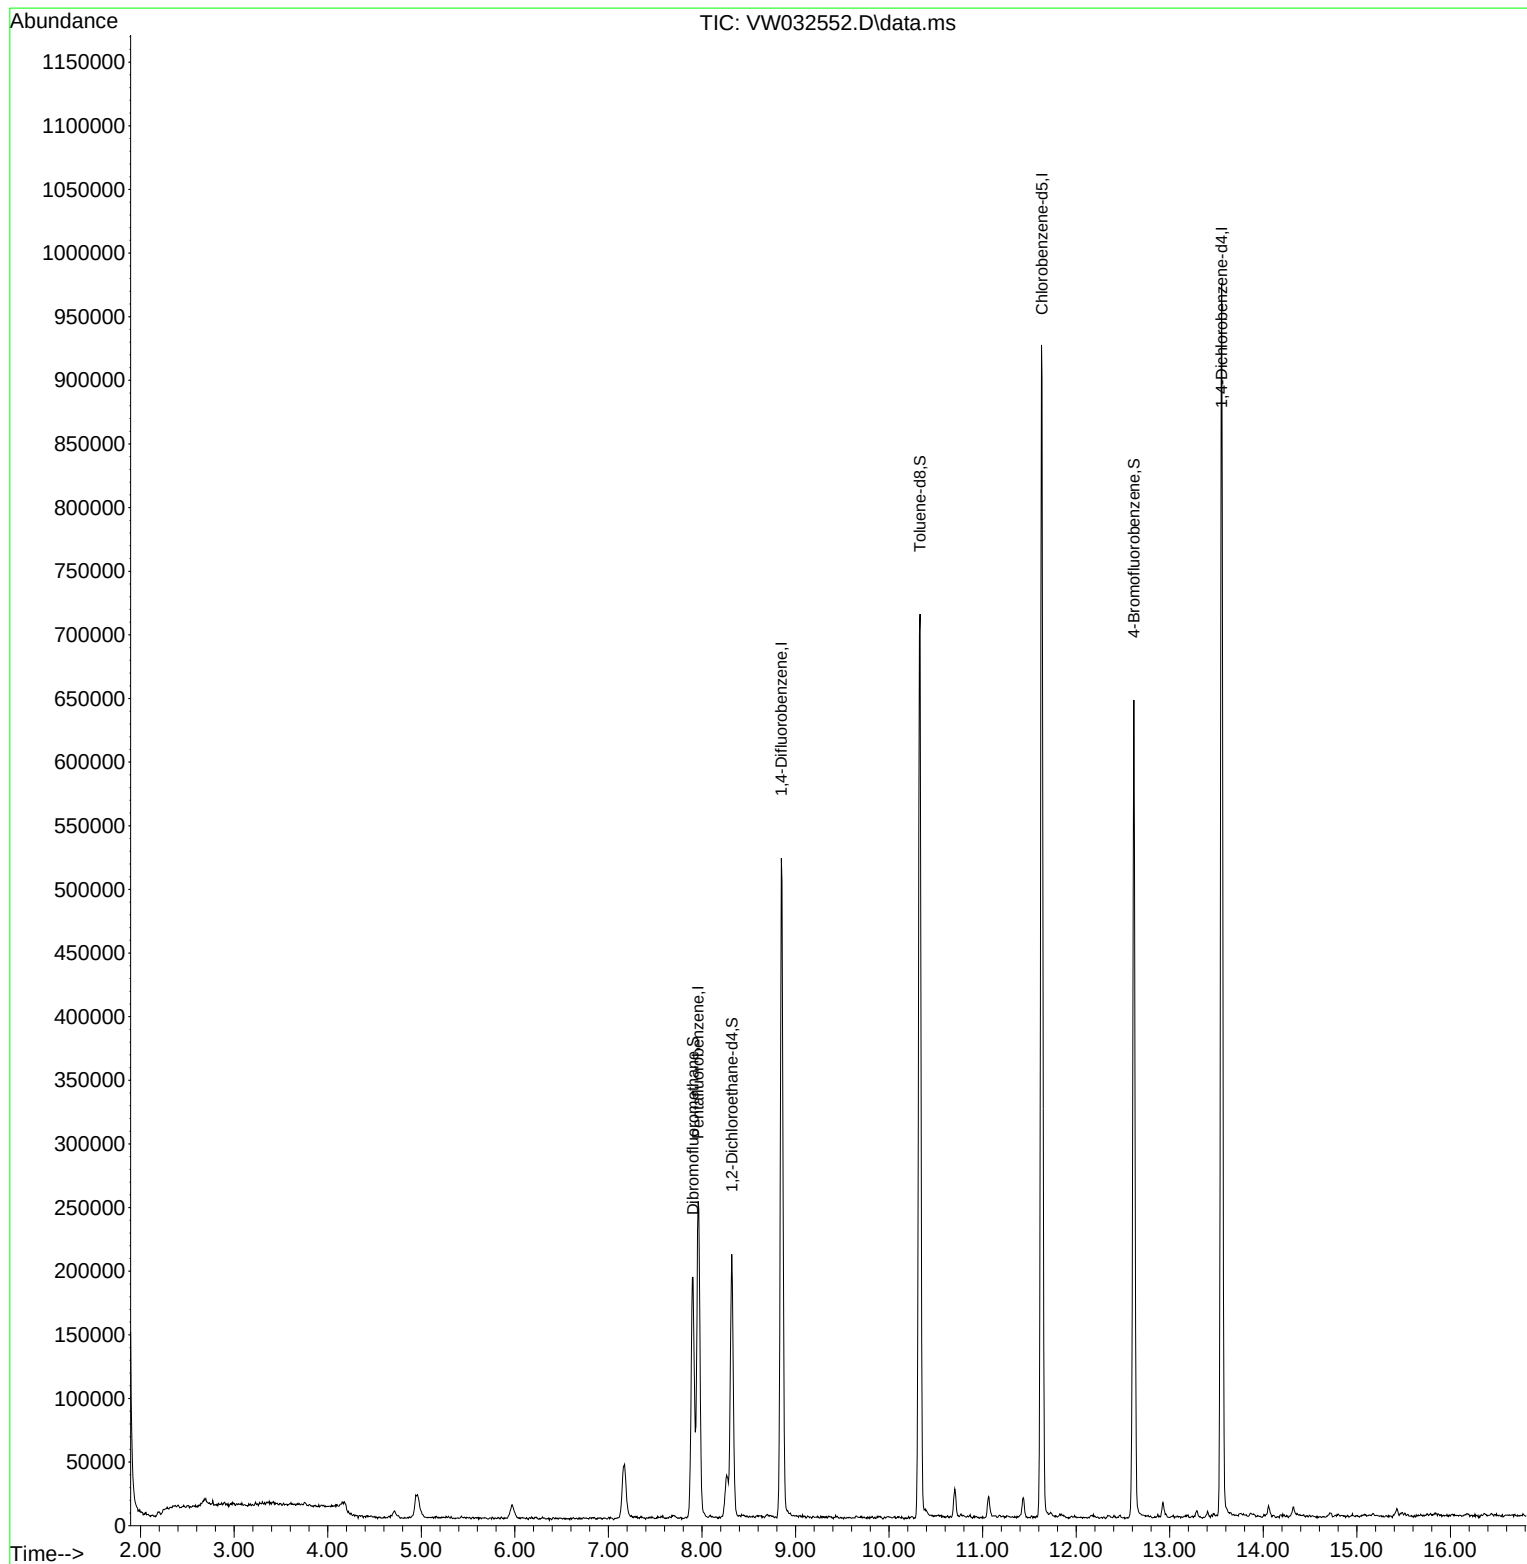


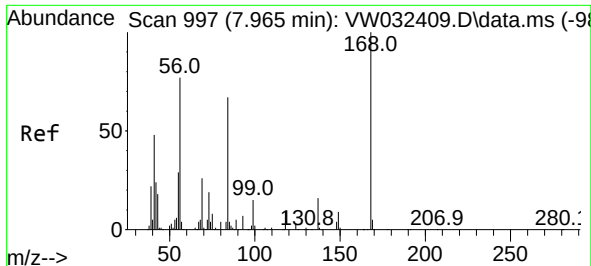

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.959 min Scan# 996
Delta R.T. -0.006 min
Lab File: VW032552.D
Acq: 26 Nov 2025 18:17




Instrument :
MSVOA_W
ClientSampleId :
SB-1125-17A


Tgt Ion:168 Resp: 171429
Ion Ratio Lower Upper
168 100
99 71.5 45.4 68.2#

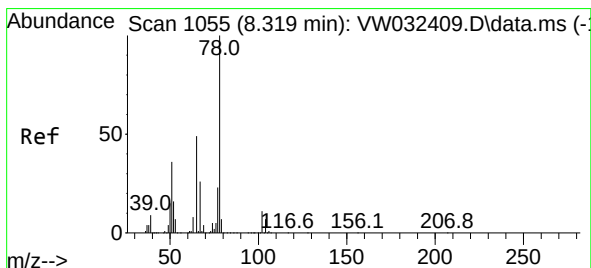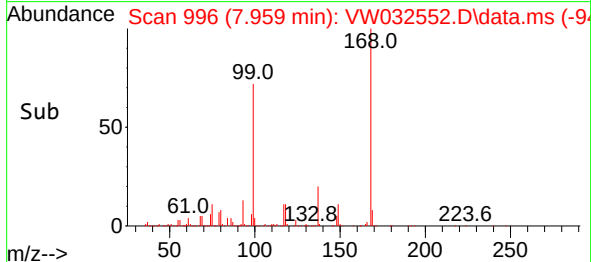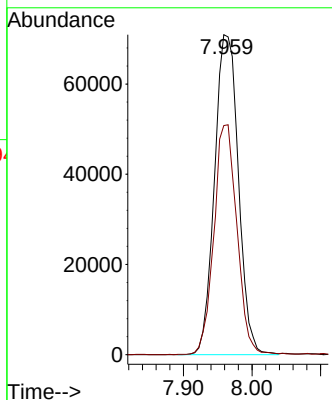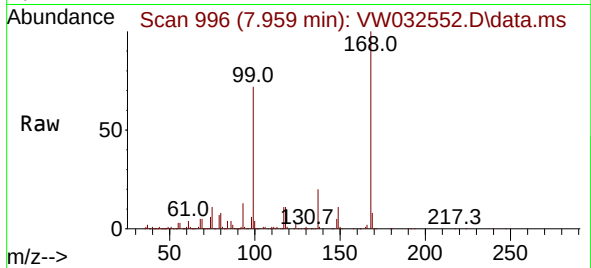

#33
1,2-Dichloroethane-d4
Concen: 74.905 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. -0.000 min
Lab File: VW032552.D
Acq: 26 Nov 2025 18:17

Tgt Ion: 65 Resp: 165549
Ion Ratio Lower Upper
65 100
67 52.1 0.0 106.8


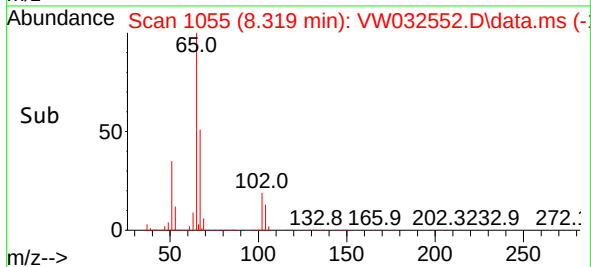
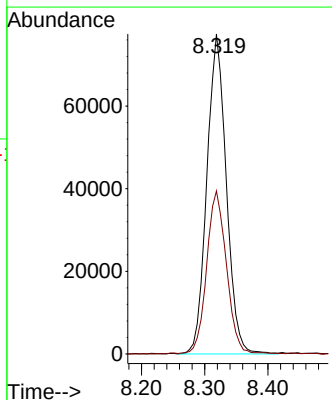
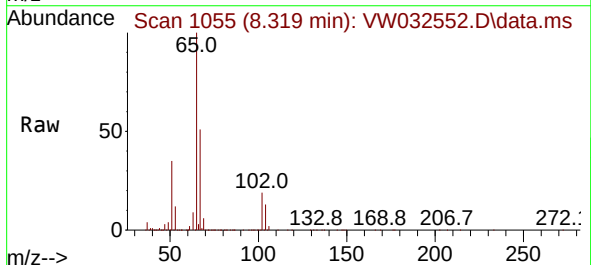


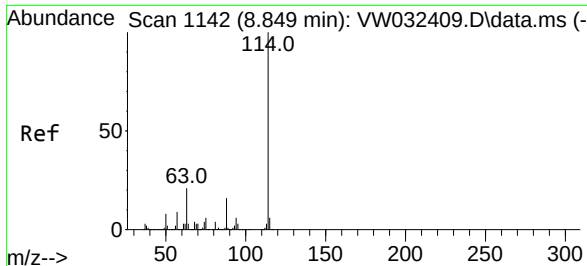

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.849 min Scan# 1142
Delta R.T. -0.000 min
Lab File: VW032552.D
Acq: 26 Nov 2025 18:17




Instrument :
MSVOA_W
ClientSampleId :
SB-1125-17A


Tgt Ion:114 Resp: 419256
Ion Ratio Lower Upper
114 100
63 23.0 0.0 41.8
88 17.4 0.0 32.6

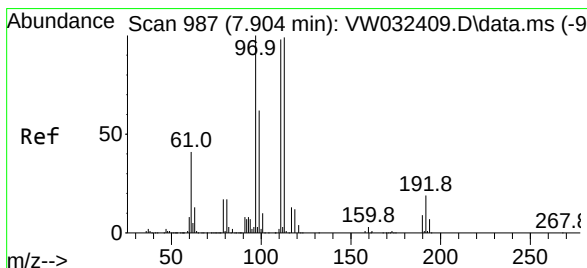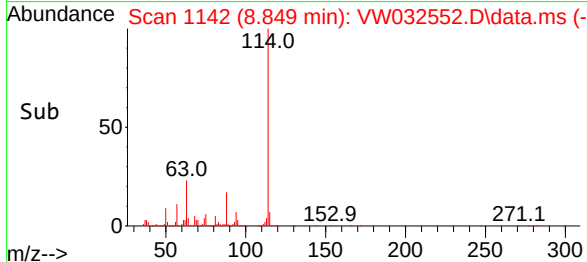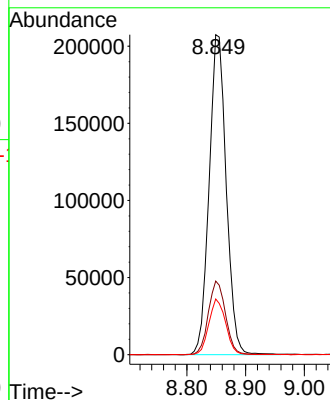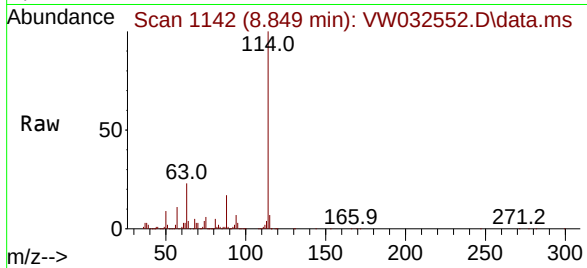

#35
Dibromofluoromethane
Concen: 55.701 ug/l
RT: 7.904 min Scan# 987
Delta R.T. -0.000 min
Lab File: VW032552.D
Acq: 26 Nov 2025 18:17

Tgt Ion:113 Resp: 139819
Ion Ratio Lower Upper
113 100
111 105.6 83.1 124.7
192 17.5 13.4 20.2


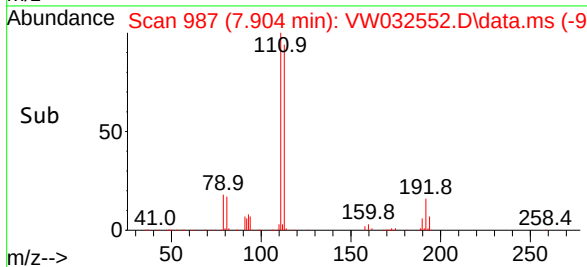
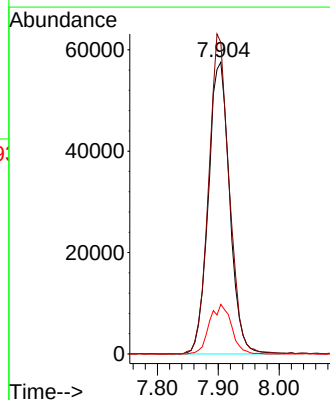
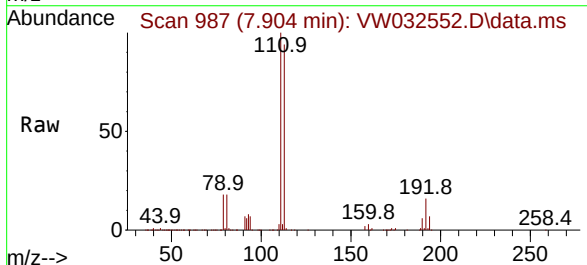


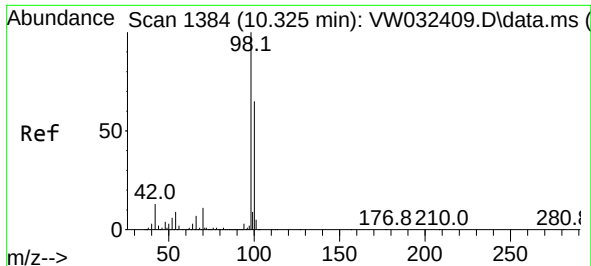

#50
Toluene-d8
Concen: 49.172 ug/l
RT: 10.330 min Scan# 11
Delta R.T. 0.006 min
Lab File: VW032552.D
Acq: 26 Nov 2025 18:17




Instrument :
MSVOA_W
ClientSampleId :
SB-1125-17A


Tgt Ion: 98 Resp: 473523
Ion Ratio Lower Upper
98 100
100 66.1 53.3 79.9

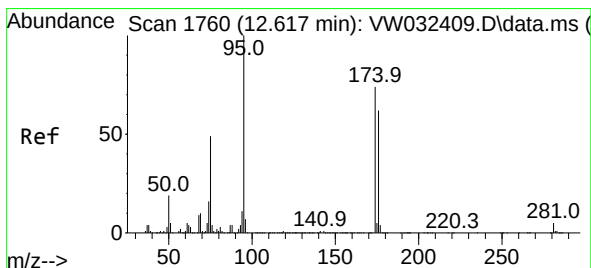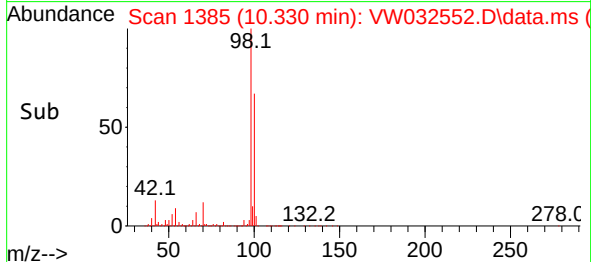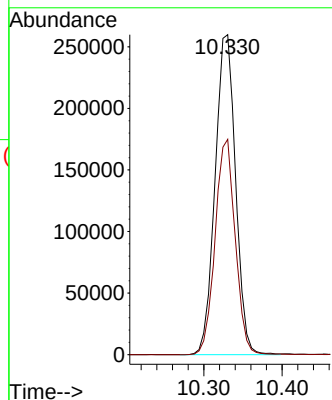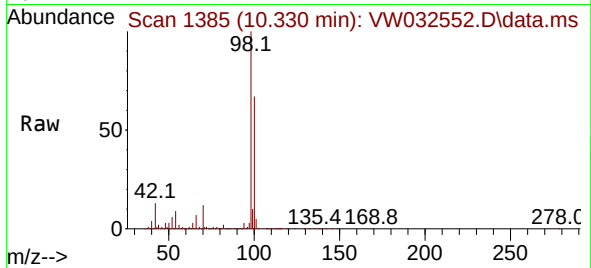

#62
4-Bromofluorobenzene
Concen: 60.282 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. -0.000 min
Lab File: VW032552.D
Acq: 26 Nov 2025 18:17

Tgt Ion: 95 Resp: 219295
Ion Ratio Lower Upper
95 100
174 66.2 0.0 135.4
176 61.6 0.0 131.8

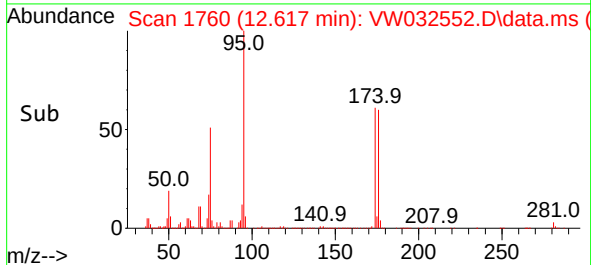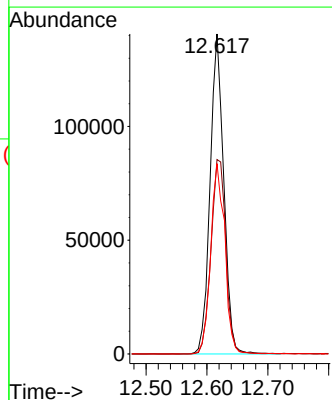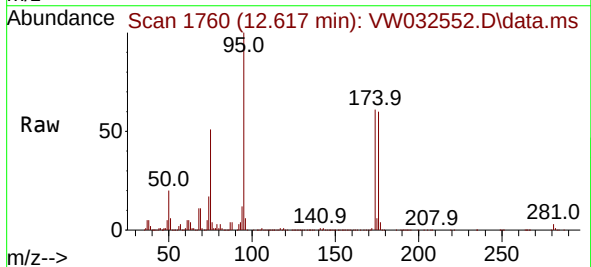

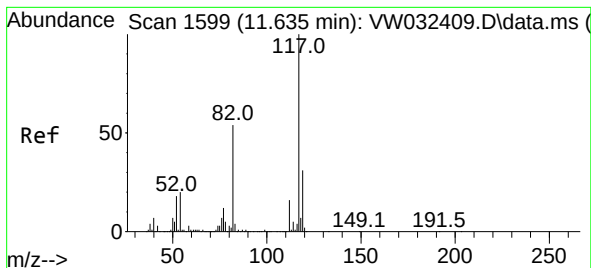

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.635 min Scan# 11

Delta R.T. -0.000 min

Lab File: VW032552.D

Acq: 26 Nov 2025 18:17

Instrument :

MSVOA_W

ClientSampleId :

SB-1125-17A





Tgt Ion:117 Resp: 506374

Ion Ratio Lower Upper

117 100

82 53.8 43.0 64.4

119 30.6 25.0 37.6

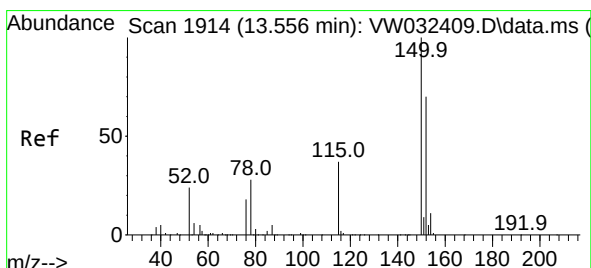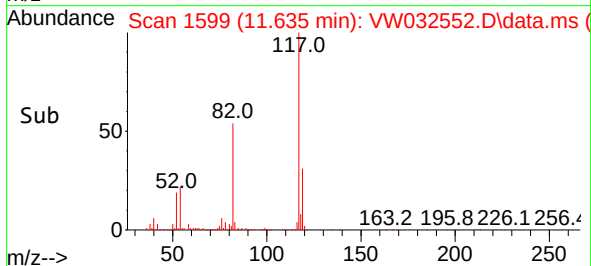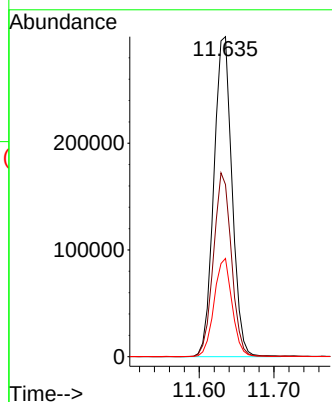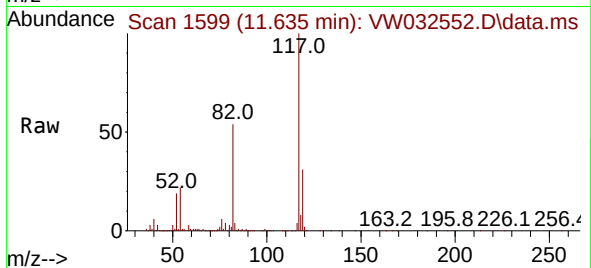

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.555 min Scan# 1914

Delta R.T. -0.000 min

Lab File: VW032552.D

Acq: 26 Nov 2025 18:17

Tgt Ion:152 Resp: 251247

Ion Ratio Lower Upper

152 100

115 64.8 32.8 98.3

150 150.2 0.0 356.6

