
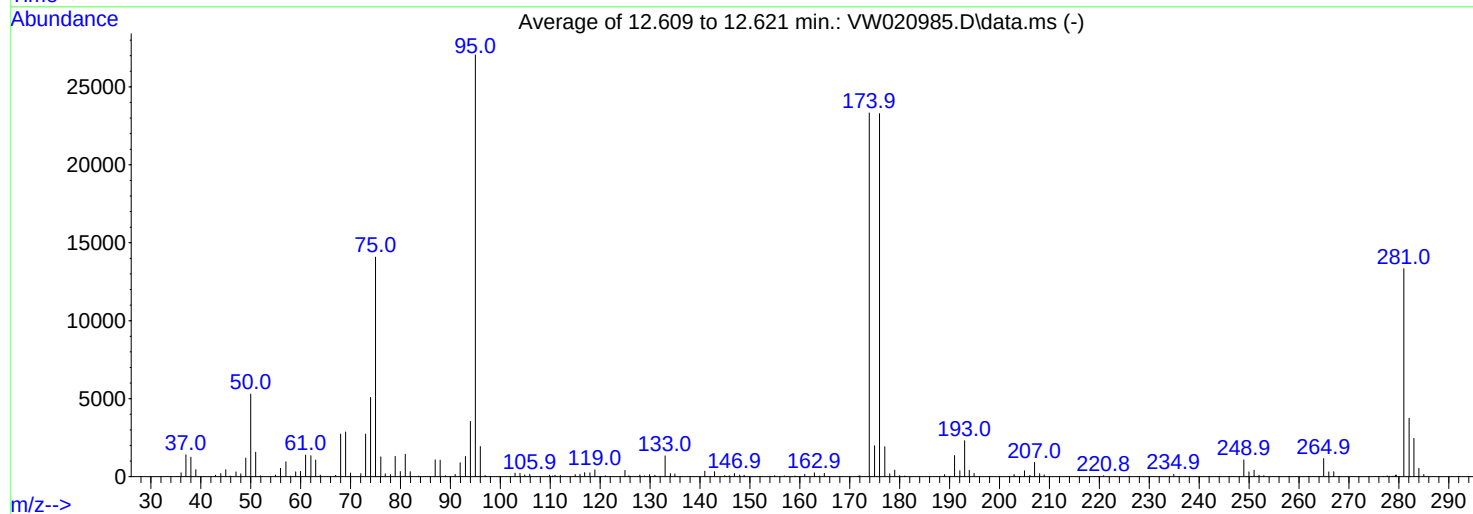


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW113021\
 Data File : VW020985.D
 Acq On : 30 Nov 2021 13:19
 Operator : SY/VA
 Sample : BFB467
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB467

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Title : SFAM01.0
 Last Update : Wed Dec 01 00:01:42 2021

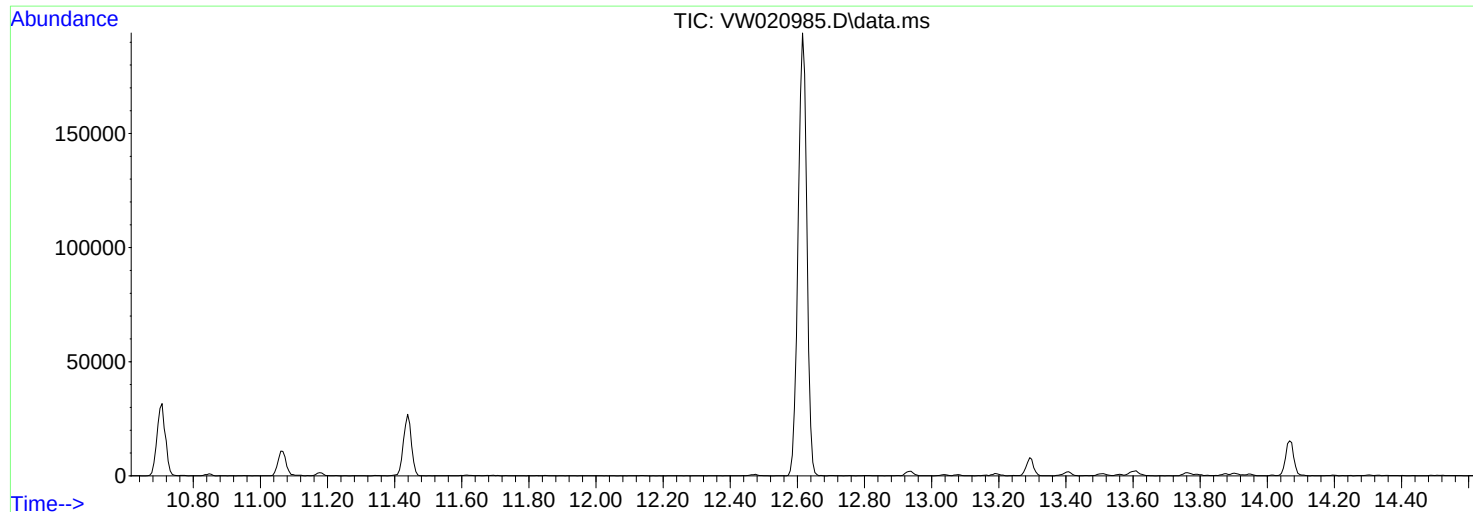

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	5295	PASS
75	95	30	80	52.0	14080	PASS
95	95	100	100	100.0	27053	PASS
96	95	5	9	7.1	1932	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.2	23326	PASS
175	174	5	9	8.5	1980	PASS
176	174	95	105	99.8	23285	PASS
177	176	5	10	8.2	1918	PASS

m/z	Abundance
36.00	244.0
37.00	1408.0
38.00	1301.0
39.00	465.0
44.00	268.0
45.00	318.0
45.80	61.0
47.00	254.0
48.00	183.0
49.00	1156.0
50.00	5398.0
51.00	1605.0
55.00	102.0
56.00	521.0
57.00	915.0
58.90	152.0
59.90	359.0
61.00	1462.0
62.00	1363.0
63.00	1126.0
64.00	103.0
67.00	83.0
68.00	2742.0
69.00	3047.0
70.10	205.0
72.10	195.0
73.00	1855.0
74.00	5267.0
75.00	14694.0
76.00	1326.0
76.90	198.0
78.10	99.0
78.90	1380.0
80.00	285.0
81.00	1527.0
81.90	346.0
87.00	1002.0
88.00	1208.0
91.00	172.0
91.90	970.0
93.00	1406.0
94.00	3630.0
95.00	29240.0
96.00	2035.0
103.10	109.0
103.90	159.0
104.90	80.0
105.90	149.0
109.80	89.0
112.10	66.0
114.90	85.0
116.00	148.0
116.90	206.0
118.00	199.0
118.80	272.0
125.10	197.0
125.90	103.0
128.00	100.0
129.90	134.0
130.90	101.0
132.90	688.0
134.10	151.0
134.80	88.0
141.00	306.0
142.10	56.0
143.00	343.0
144.90	104.0
145.90	65.0
146.80	108.0
147.90	102.0
148.90	60.0
155.00	61.0
156.90	63.0
159.00	52.0
161.00	111.0
162.90	107.0
165.00	95.0
172.00	111.0
173.90	28752.0
175.00	2260.0
175.90	29600.0
177.00	1971.0
178.00	103.0
179.00	204.0
180.00	57.0
188.90	77.0
191.00	732.0
192.00	173.0
193.00	1215.0
193.90	209.0
195.00	146.0
203.10	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB467

205.00	187.0
207.00	424.0
208.00	147.0
208.80	54.0
234.90	130.0
248.90	698.0
249.90	155.0
251.00	263.0
252.10	56.0
264.90	670.0
266.00	184.0
267.00	273.0
278.80	96.0
281.00	5812.0
282.00	2650.0
283.00	1638.0
284.00	359.0
285.00	120.0

Instrument :
MSVOA_W
ClientSampleId :
BFB467

m/z	Abundance
41.00	63.0
44.00	85.0
280.90	76.0
281.20	82.0

Instrument :
MSVOA_W
ClientSampleId :
BFB467

m/z	Abundance
36.10	201.0
37.00	1222.0
38.00	1181.0
39.00	391.0
43.00	171.0
44.00	241.0
45.00	606.0
47.00	369.0
48.00	152.0
49.00	1091.0
50.00	4757.0
51.00	1439.0
51.90	75.0
55.00	104.0
56.00	477.0
57.10	921.0
58.00	78.0
59.00	498.0
60.00	292.0
61.00	1191.0
62.10	1106.0
63.00	907.0
63.90	105.0
67.10	60.0
68.00	2325.0
69.00	2286.0
69.90	244.0
72.00	175.0
73.00	3527.0
74.00	4520.0
75.00	11767.0
76.00	1176.0
76.90	124.0
77.90	96.0
78.90	1130.0
79.90	280.0
80.90	1249.0
82.00	256.0
85.00	50.0
86.90	1128.0
88.00	784.0
89.00	174.0
90.90	125.0
91.90	634.0
93.00	1069.0
94.00	2999.0
95.00	21192.0
96.00	1703.0
97.00	119.0
102.90	309.0
103.90	260.0
104.90	113.0
105.90	143.0
109.90	95.0
110.50	130.0
110.90	132.0
111.90	105.0
115.00	198.0
115.90	183.0
116.90	307.0
117.90	298.0
119.00	592.0
120.00	50.0
121.00	97.0
125.00	682.0
127.90	85.0
128.90	65.0
129.90	93.0
130.90	91.0
132.00	88.0
133.00	2059.0
134.00	444.0
134.90	265.0
140.90	341.0
142.80	285.0
145.00	53.0
145.90	65.0
147.00	319.0
147.90	97.0
148.90	142.0
155.00	60.0
161.00	211.0
162.90	378.0
164.00	67.0
164.90	327.0
172.00	81.0
173.90	15002.0
174.90	1543.0
176.00	16744.0
177.00	1914.0
178.00	280.0
179.00	548.0

Instrument :
MSVOA_W
ClientSampleId :
BFB467

179.90	83.0
181.00	58.0
189.10	163.0
191.00	2213.0
192.10	563.0
193.00	3175.0
194.00	585.0
195.00	281.0
202.90	278.0
205.00	633.0
206.20	148.0
207.00	1410.0
208.10	272.0
208.90	170.0
219.00	53.0
220.80	87.0
234.90	217.0
237.20	65.0
249.00	1390.0
249.90	400.0
251.00	562.0
252.00	146.0
253.00	110.0
264.90	1596.0
266.00	392.0
266.90	295.0
268.10	58.0
276.90	66.0
277.70	62.0
279.30	288.0
281.00	19384.0
282.10	5193.0
283.00	3115.0
284.00	691.0
285.00	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB467

m/z	Abundance
36.00	294.0
37.00	1591.0
38.00	1265.0
39.00	501.0
42.90	99.0
44.00	326.0
45.00	408.0
45.90	52.0
47.10	307.0
48.00	209.0
49.00	1333.0
50.00	5730.0
51.00	1679.0
52.00	90.0
54.90	111.0
55.90	618.0
57.00	1035.0
59.00	270.0
60.00	367.0
61.00	1493.0
62.00	1575.0
63.00	1177.0
63.90	88.0
66.90	96.0
68.00	3121.0
69.00	3246.0
70.00	273.0
72.00	222.0
73.00	2802.0
74.00	5450.0
75.00	15780.0
76.10	1318.0
77.00	230.0
78.00	196.0
79.00	1404.0
79.90	425.0
81.00	1534.0
82.00	362.0
83.60	81.0
87.00	1092.0
87.90	1171.0
90.90	144.0
92.00	1085.0
93.00	1418.0
94.00	3997.0
95.00	30728.0
96.00	2058.0
96.90	89.0
103.00	246.0
104.00	228.0
104.90	134.0
105.90	185.0
109.90	99.0
111.00	146.0
112.00	88.0
115.00	116.0
116.00	136.0
116.90	246.0
118.00	249.0
119.00	467.0
121.10	59.0
124.90	332.0
125.70	166.0
127.90	117.0
128.90	85.0
129.90	136.0
131.00	89.0
133.00	1261.0
135.00	184.0
140.90	388.0
142.90	340.0
144.90	63.0
145.80	69.0
146.90	193.0
148.00	99.0
148.80	85.0
154.90	61.0
156.90	78.0
159.00	61.0
161.00	132.0
162.90	240.0
163.90	54.0
164.90	230.0
171.70	79.0
173.90	26224.0
175.00	2136.0
175.90	23512.0
177.00	1870.0
178.00	168.0
179.00	501.0
179.90	59.0
181.00	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB467

189.00	163.0
190.10	87.0
191.00	1132.0
192.00	418.0
193.00	2547.0
193.90	423.0
194.80	211.0
202.90	147.0
204.10	75.0
205.00	310.0
206.00	111.0
207.00	901.0
208.00	170.0
209.00	141.0
220.90	106.0
234.90	115.0
248.90	1147.0
250.00	373.0
251.00	392.0
251.90	87.0
252.90	80.0
265.00	1214.0
265.90	336.0
267.00	392.0
277.60	95.0
278.20	81.0
279.50	302.0
281.00	15307.0
282.00	3385.0
283.00	2618.0
284.00	546.0
285.00	201.0

Instrument :
MSVOA_W
ClientSampleId :
BFB467