
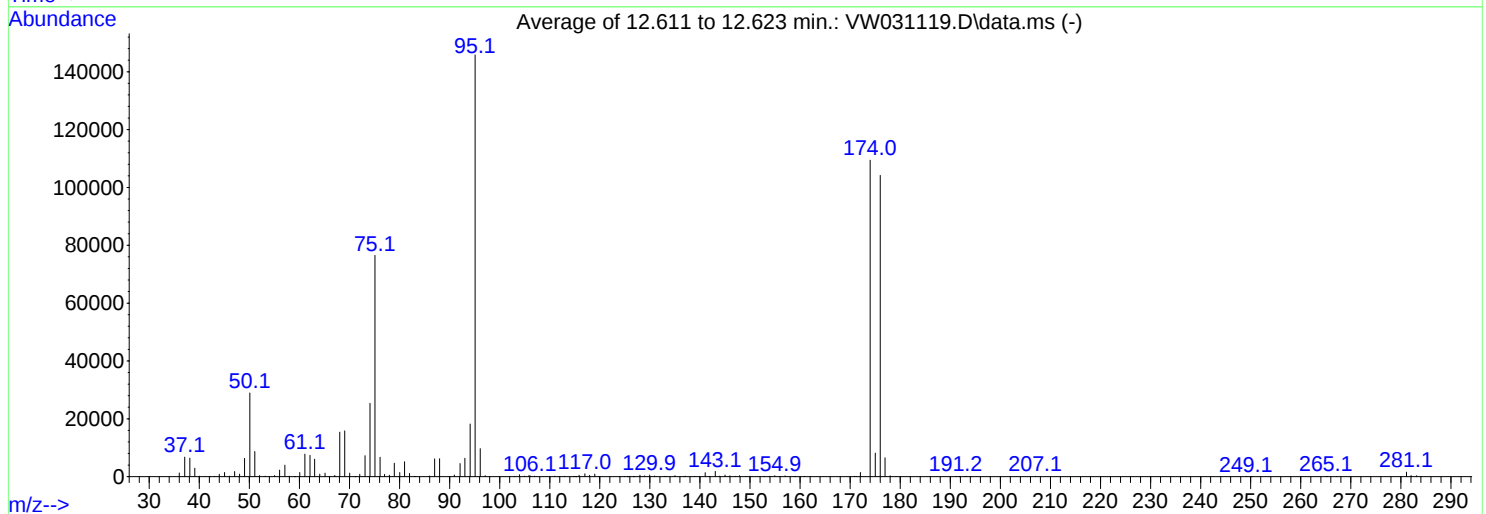


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120424\
Data File : VW031119.D
Acq On : 04 Dec 2024 08:26
Operator : SY/MD
Sample : BFB407
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB407

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Title : SFAM01.0
Last Update : Thu Dec 05 01:31:20 2024

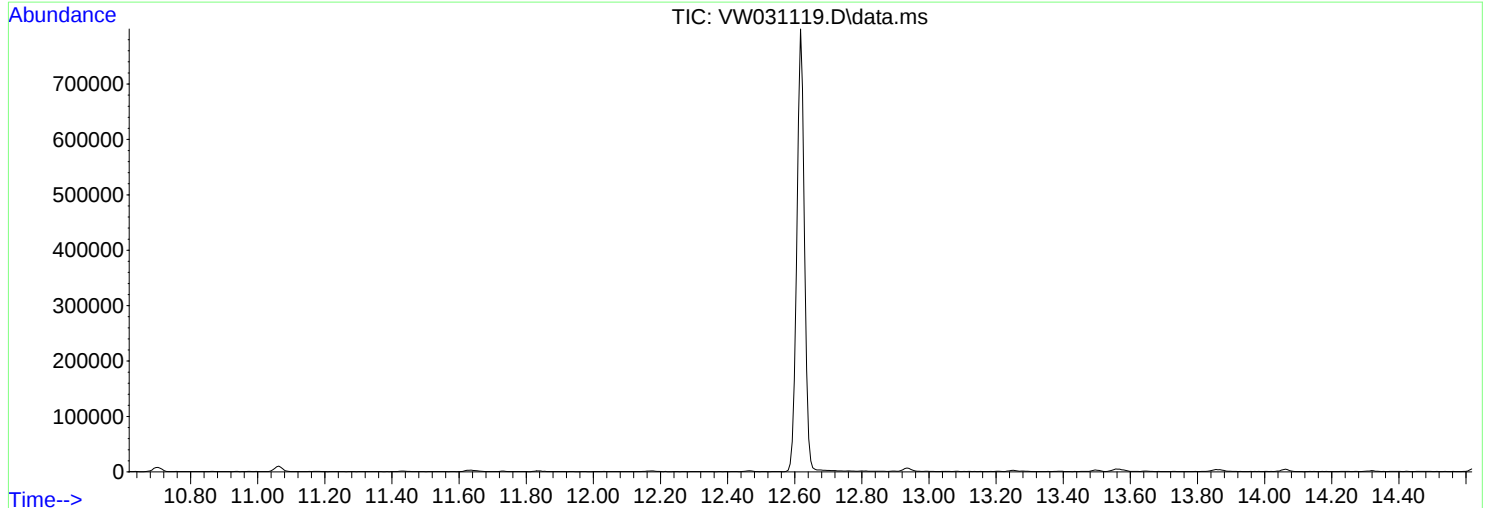

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	28965	PASS
75	95	30	80	52.5	76515	PASS
95	95	100	100	100.0	145856	PASS
96	95	5	9	6.6	9672	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.0	109448	PASS
175	174	5	9	7.4	8151	PASS
176	174	95	101	95.2	104160	PASS
177	176	5	9	6.3	6531	PASS

Scan 1751 (12.562 min): VW031119.D\data.ms
BFB407

m/z	Abundance
36.90	68.0
39.90	176.0
44.00	185.0

Instrument :
MSVOA_W
ClientSampleId :
BFB407

m/z	Abundance
36.00	1250.0
37.10	6635.0
38.10	6267.0
39.10	3098.0
40.00	351.0
43.00	117.0
44.00	1004.0
45.10	1405.0
46.00	212.0
47.00	1591.0
48.00	755.0
49.10	6391.0
50.10	28312.0
51.10	8392.0
52.10	358.0
53.20	152.0
54.10	71.0
55.10	393.0
56.10	2145.0
57.10	3768.0
57.90	211.0
59.00	57.0
60.10	1452.0
61.10	7485.0
62.10	7061.0
63.10	5890.0
64.10	1028.0
65.10	1373.0
66.00	111.0
67.00	323.0
68.00	15156.0
69.10	14649.0
70.10	1293.0
71.10	62.0
72.00	926.0
73.10	6879.0
74.10	23656.0
75.10	72576.0
76.10	6161.0
77.00	576.0
77.90	485.0
78.90	4405.0
80.10	1365.0
81.00	4681.0
82.00	953.0
83.00	140.0
85.90	335.0
87.00	6022.0
88.00	5381.0
91.00	548.0
92.10	4134.0
93.00	5899.0
94.10	15768.0
95.10	134592.0
96.10	9348.0
97.10	332.0
103.00	126.0
104.00	564.0
105.00	213.0
105.90	712.0
106.90	200.0
109.90	116.0
111.10	144.0
111.90	85.0
113.10	118.0
114.80	203.0
115.90	477.0
117.00	844.0
117.90	396.0
119.00	783.0
119.90	59.0
124.00	73.0
125.00	163.0
126.00	91.0
128.10	469.0
128.90	251.0
129.90	542.0
130.90	192.0
133.00	328.0
135.00	256.0
137.10	201.0
138.90	135.0
139.80	191.0
141.10	1182.0
143.10	1806.0
144.10	160.0
145.10	761.0
146.00	171.0
147.10	102.0
147.90	346.0
150.10	172.0
152.90	155.0

Instrument :
MSVOA_W
ClientSampleId :
BFB407

153.80	68.0
154.90	304.0
157.10	189.0
158.80	260.0
161.00	124.0
170.90	228.0
172.00	1665.0
174.00	78760.0
175.00	7417.0
176.00	89376.0
177.00	5869.0
178.00	316.0
179.10	102.0
180.00	53.0
191.20	193.0
191.80	74.0
193.20	337.0
194.00	66.0
207.00	221.0
249.10	114.0
250.10	74.0
265.10	353.0
267.20	123.0
281.10	2322.0
282.00	531.0
283.20	362.0
284.10	99.0

Instrument :
MSVOA_W
ClientSampleId :
BFB407

m/z	Abundance
36.00	1347.0
37.10	7423.0
38.10	6855.0
39.10	3249.0
40.10	347.0
41.20	144.0
42.90	77.0
44.10	1166.0
45.10	1559.0
46.00	107.0
47.10	1880.0
48.10	1085.0
49.10	6890.0
50.10	32256.0
51.10	9914.0
52.10	438.0
53.10	160.0
54.00	110.0
55.00	512.0
56.10	2579.0
57.10	4534.0
58.00	171.0
60.00	1610.0
61.10	8616.0
62.10	8483.0
63.10	7008.0
64.00	897.0
65.10	1430.0
66.00	156.0
67.00	484.0
68.10	16720.0
69.10	18048.0
70.10	1367.0
72.00	865.0
73.10	8526.0
74.10	28752.0
75.10	83704.0
76.10	7942.0
77.00	809.0
77.90	636.0
79.00	5156.0
80.00	1623.0
81.00	6033.0
82.00	1314.0
83.20	140.0
86.00	245.0
87.00	6725.0
88.00	7101.0
91.00	642.0
92.10	5419.0
93.10	7465.0
94.10	20792.0
95.10	166208.0
96.10	11003.0
97.10	402.0
103.00	142.0
103.90	745.0
104.90	214.0
106.10	656.0
107.00	110.0
110.00	127.0
110.90	211.0
111.90	92.0
112.90	163.0
115.00	184.0
115.90	569.0
117.00	1104.0
118.00	564.0
118.90	930.0
119.80	96.0
125.50	91.0
126.00	113.0
126.70	65.0
128.00	614.0
128.90	328.0
130.00	506.0
130.90	279.0
133.20	204.0
135.00	479.0
137.00	385.0
139.00	85.0
139.90	101.0
141.00	1621.0
142.00	247.0
143.00	2108.0
143.90	124.0
144.90	588.0
145.90	337.0
147.00	123.0
147.80	292.0
149.10	121.0
149.90	179.0

Instrument :
MSVOA_W
ClientSampleId :
BFB407

152.90	110.0
153.80	116.0
155.00	477.0
155.90	131.0
156.90	390.0
159.00	153.0
160.80	153.0
170.00	59.0
171.20	234.0
172.10	1455.0
174.00	127544.0
175.00	10055.0
176.00	113664.0
176.90	7144.0
178.00	320.0
179.20	78.0
180.00	56.0
191.10	106.0
192.90	180.0
207.10	119.0
249.10	82.0
265.30	158.0
267.00	85.0
281.10	1456.0
282.10	499.0
283.10	372.0
284.20	75.0

Instrument :
MSVOA_W
ClientSampleId :
BFB407

m/z	Abundance
36.00	1184.0
37.10	6164.0
38.10	6115.0
39.10	2432.0
40.00	365.0
41.10	81.0
42.00	70.0
43.10	95.0
44.10	967.0
45.00	1349.0
46.10	253.0
47.10	1846.0
48.00	901.0
49.00	5651.0
50.10	26328.0
51.10	7750.0
52.00	336.0
53.10	132.0
54.00	78.0
55.00	346.0
56.00	2077.0
57.10	3594.0
58.00	148.0
60.00	1236.0
61.10	7237.0
62.10	6519.0
63.00	5260.0
64.00	829.0
65.10	924.0
66.10	149.0
67.10	481.0
68.10	14324.0
69.00	14771.0
70.00	1037.0
72.10	768.0
73.10	6366.0
74.10	23696.0
75.10	73264.0
76.10	5936.0
77.00	923.0
78.00	417.0
79.00	4369.0
80.00	1377.0
81.00	4697.0
82.00	1051.0
83.00	146.0
85.90	149.0
87.00	5758.0
88.00	6172.0
90.90	492.0
92.10	4112.0
93.00	5808.0
94.10	18016.0
95.10	136768.0
96.10	8665.0
97.10	217.0
102.90	68.0
104.00	709.0
105.00	167.0
105.80	633.0
106.90	208.0
110.00	97.0
111.00	173.0
111.80	81.0
112.90	119.0
114.70	91.0
115.20	76.0
115.80	525.0
117.00	1010.0
117.90	400.0
119.10	898.0
119.90	52.0
123.90	126.0
124.90	97.0
126.00	106.0
127.90	423.0
129.00	249.0
130.00	586.0
131.00	182.0
133.20	87.0
134.90	215.0
136.80	208.0
139.00	64.0
139.90	115.0
141.00	1422.0
141.80	133.0
143.00	1539.0
143.80	151.0
145.00	394.0
146.00	293.0
147.00	121.0
148.00	397.0

Instrument :
MSVOA_W
ClientSampleId :
BFB407

149.20	112.0
150.00	141.0
152.90	114.0
153.90	185.0
154.90	270.0
155.90	97.0
157.10	264.0
159.10	198.0
160.80	143.0
170.10	66.0
170.90	163.0
172.00	1290.0
174.00	122040.0
175.00	6980.0
176.00	109440.0
176.90	6581.0
178.00	199.0
191.00	54.0
249.10	81.0
265.00	63.0
281.10	855.0
282.10	225.0
283.20	231.0

Instrument :
MSVOA_W
ClientSampleId :
BFB407