



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120525\
Data File : VW032571.D
Acq On : 05 Dec 2025 08:15
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W120325S.M
Title : SW846 8260
Last Update : Thu Dec 04 04:04:32 2025

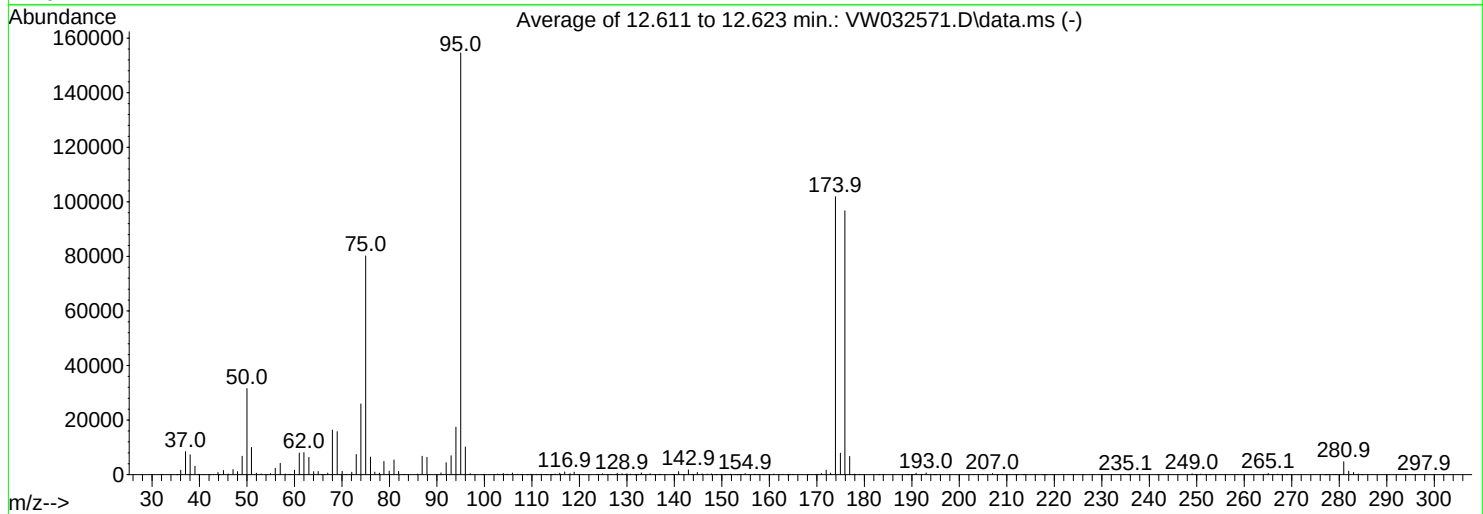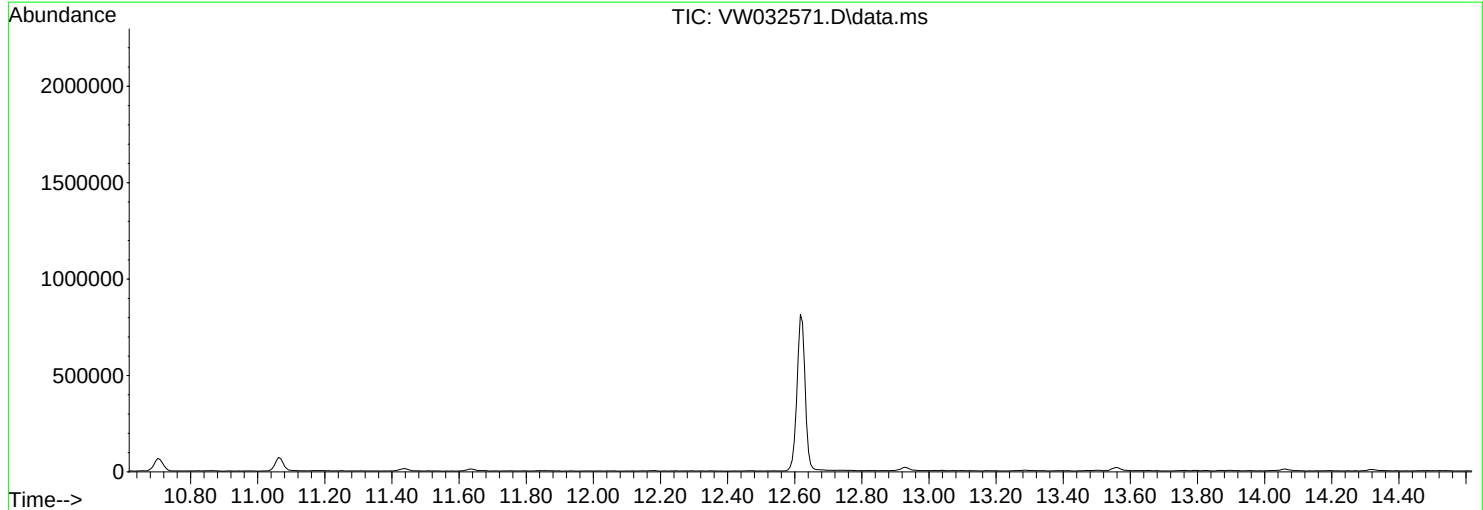

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	31530	PASS
75	95	30	60	51.8	80165	PASS
95	95	100	100	100.0	154611	PASS
96	95	5	9	6.6	10150	PASS
173	174	0.00	2	0.6	578	PASS
174	95	50	100	65.9	101848	PASS
175	174	5	9	7.7	7835	PASS
176	174	95	101	94.9	96688	PASS
177	176	5	9	6.9	6669	PASS