

Data File : VW014245.D
Acq On : 06 Dec 2019 13:19
Operator : SY/VA
Sample : K6149-13
Misc : 5.69G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBBS7

Quant Time: Dec 07 04:13:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 04:10:05 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1278085	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1154632	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	509122	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	471458	24.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.44%
7) Chloroethane-d5	2.89	69	344283	23.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.68%
10) 1,1-Dichloroethene-d2	4.02	63	620480	18.15	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.60%
20) 2-Butanone-d5	7.07	46	173399	34.38	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.76%
24) Chloroform-d	7.65	84	738169	22.68	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.72%
26) 1,2-Dichloroethane-d4	8.30	65	377765	22.14	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.56%
29) Benzene-d6	8.27	84	1605015	23.72	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.88%
33) 1,2-Dichloropropane-d6	9.27	67	482375	23.17	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.68%
37) Toluene-d8	10.32	98	1449177	23.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.72%
38) trans-1,3-Dichloropropene-	10.57	79	181086	20.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.92%
39) 2-Hexanone-d5	10.92	63	133629	32.28	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.56%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	320485	18.89	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	75.56%
61) 1,2-Dichlorobenzene-d4	13.85	152	462074	23.75	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.00%


Target Compounds					Qvalue
42) cis-1,3-Dichloropropene	10.03	75	11471	0.408 ug/L	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014245.D
Acq On : 06 Dec 2019 13:19
Operator : SY/VA
Sample : K6149-13
Misc : 5.69G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBBS7

Quant Time: Dec 07 04:13:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 07 04:10:05 2019
Response via : Initial Calibration

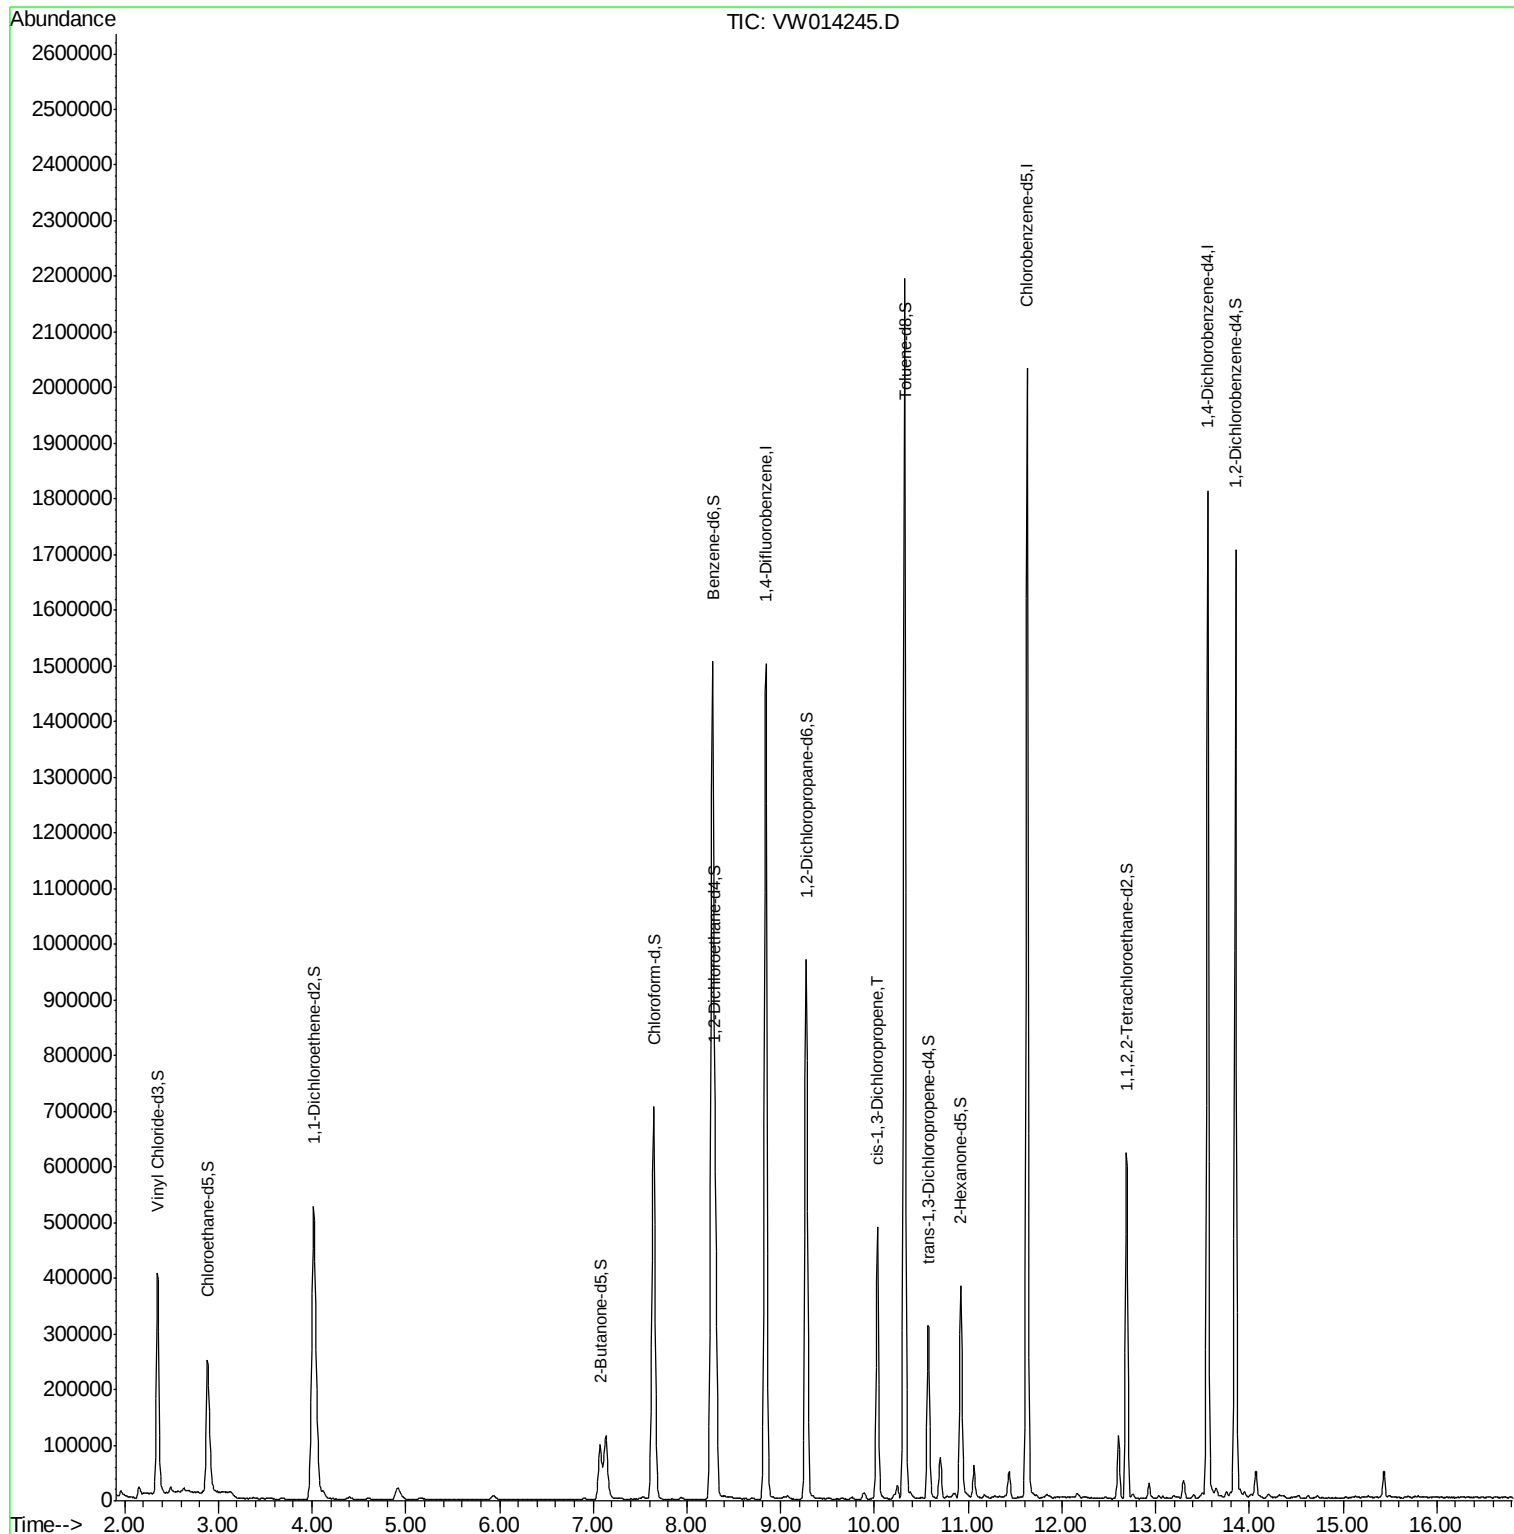

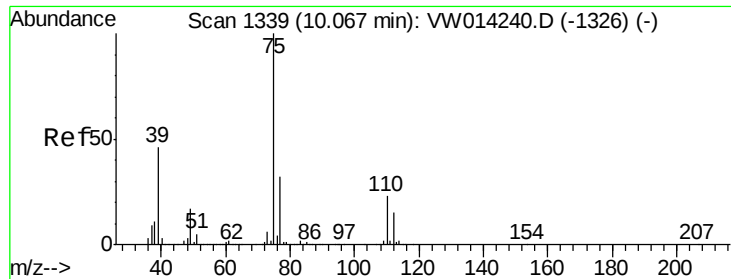

#42

cis-1,3-Dichloropropene

Concen: 0.408 ug/L

RT: 10.03 min Scan# 1333

Delta R.T. -0.04 min

Lab File: VW014245.D

Acq: 06 Dec 2019 13:19

Instrument :

MSVOA_W

ClientSampleId :

DBBS7

Tgt Ion: 75 Resp: 11471

Ion Ratio Lower Upper

75 100

77 54.2 22.1 41.1#

